

Technical validation of patient-specific expressed proteome reconstruction

Cohort-level metrics derived from Amylice reconstructed proteomes and prediction-ready outputs.

Samples processed

8

8 complete, 0 incomplete

Median sequences

24,138

reconstructed per sample

Median frameshifts

446


altered protein products

Median retained


99.9%

after prediction merge


A Reconstructed protein sequences per sample

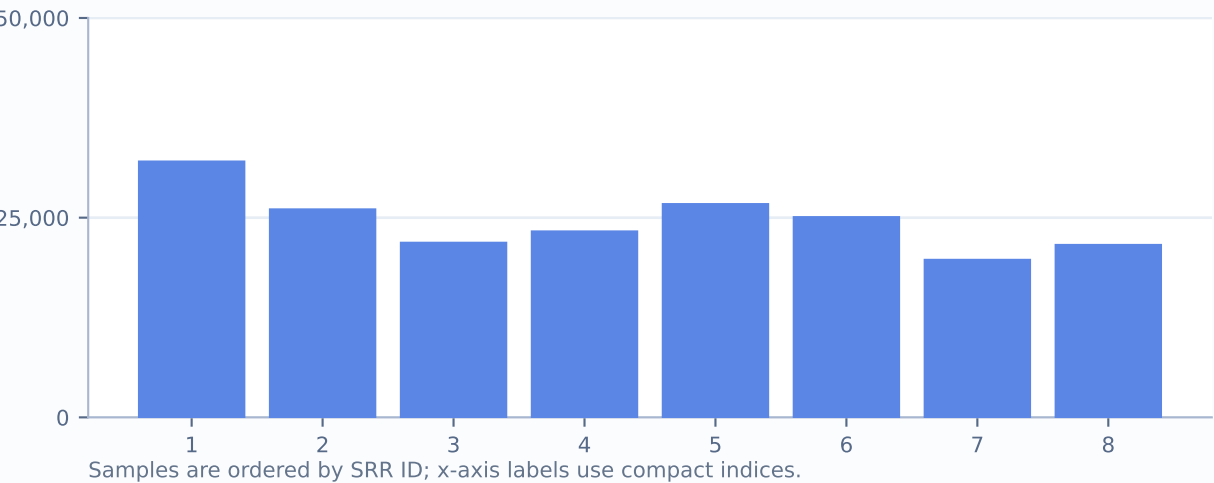


B Proteoform classes in each reconstructed proteome

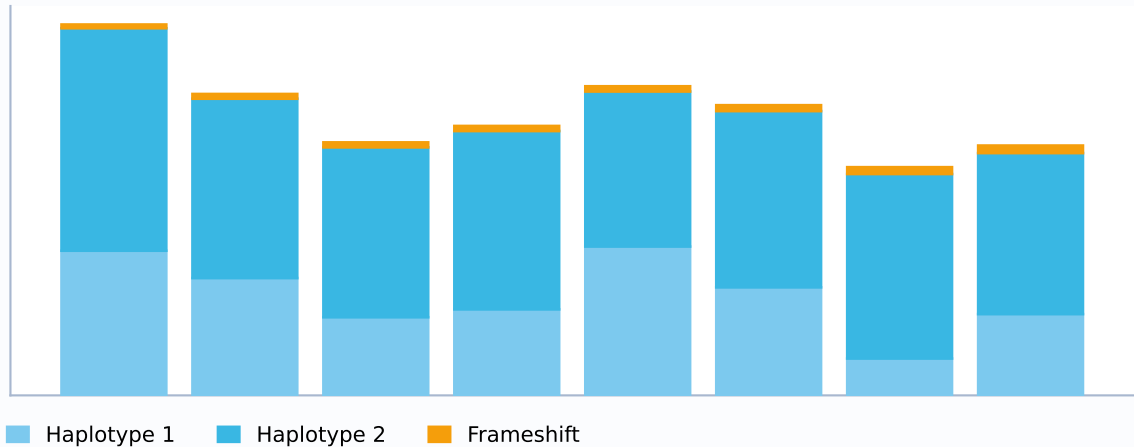

C Protein length distribution

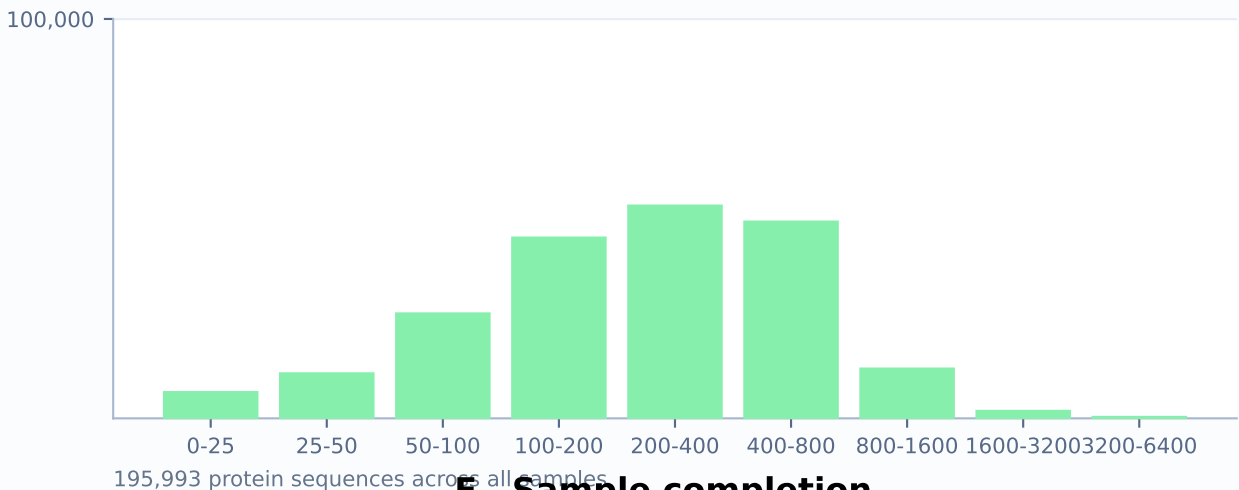

D Prediction-ready retained fraction

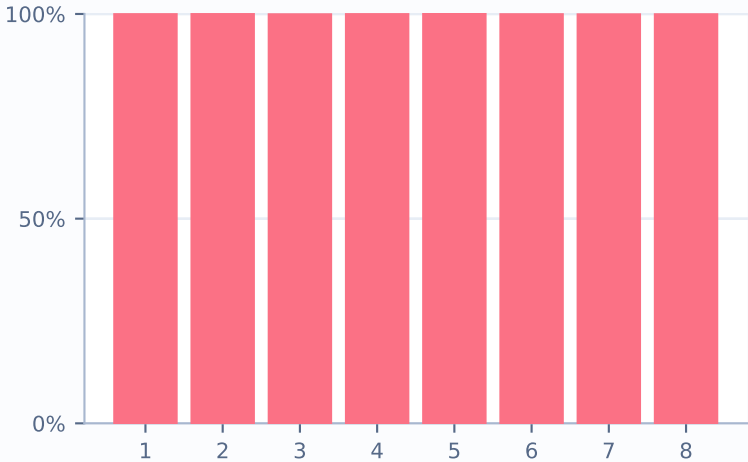

F Sample index

	sample	sequences
1	SRR32060218	31,992
2	SRR32060222	26,001
3	SRR32060224	21,824
4	SRR32060226	23,242
5	SRR32060252	26,665
6	SRR32060255	25,033
7	SRR32060299	19,685
8	SRR32060304	21,551

E Sample completion



8/8

Completed samples: 8