
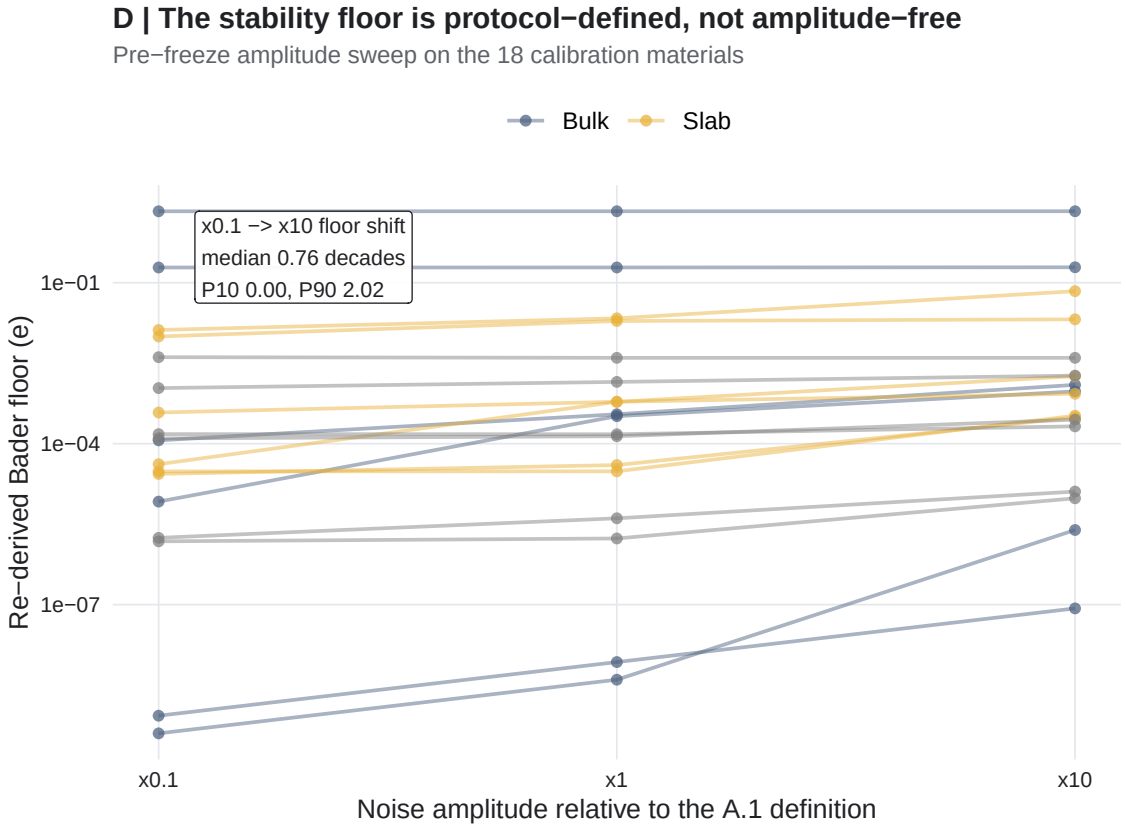
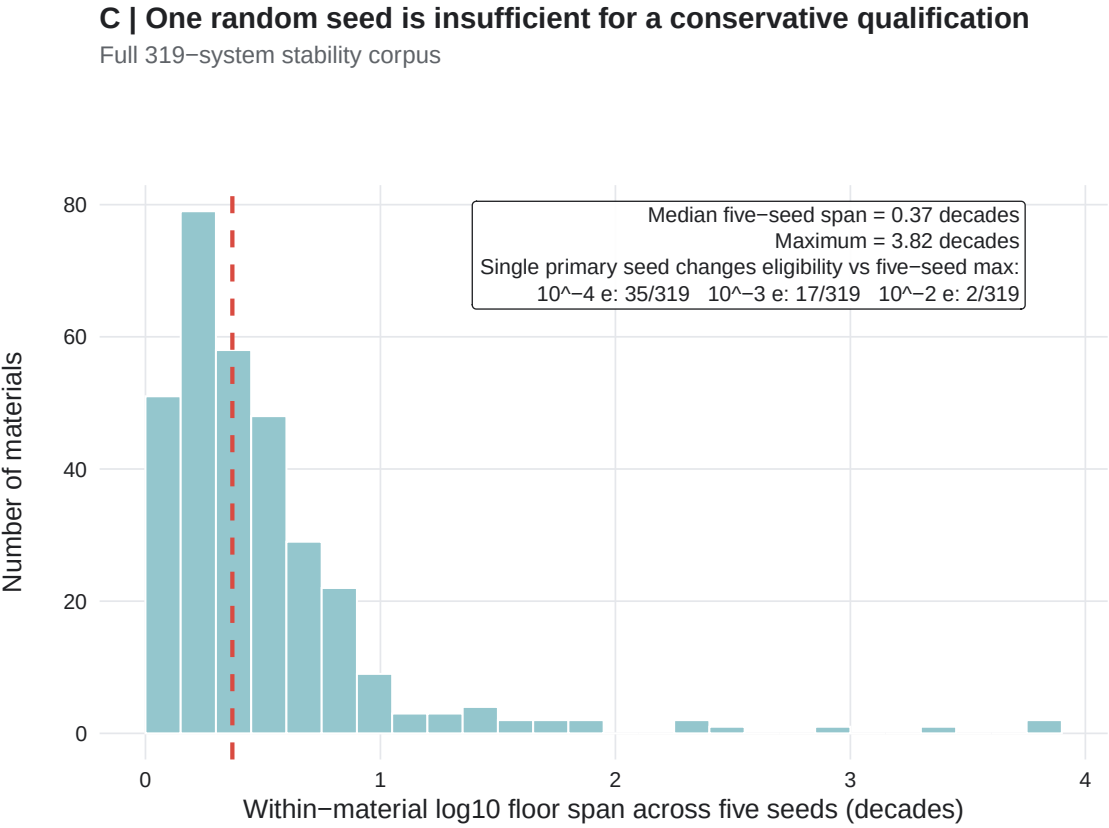
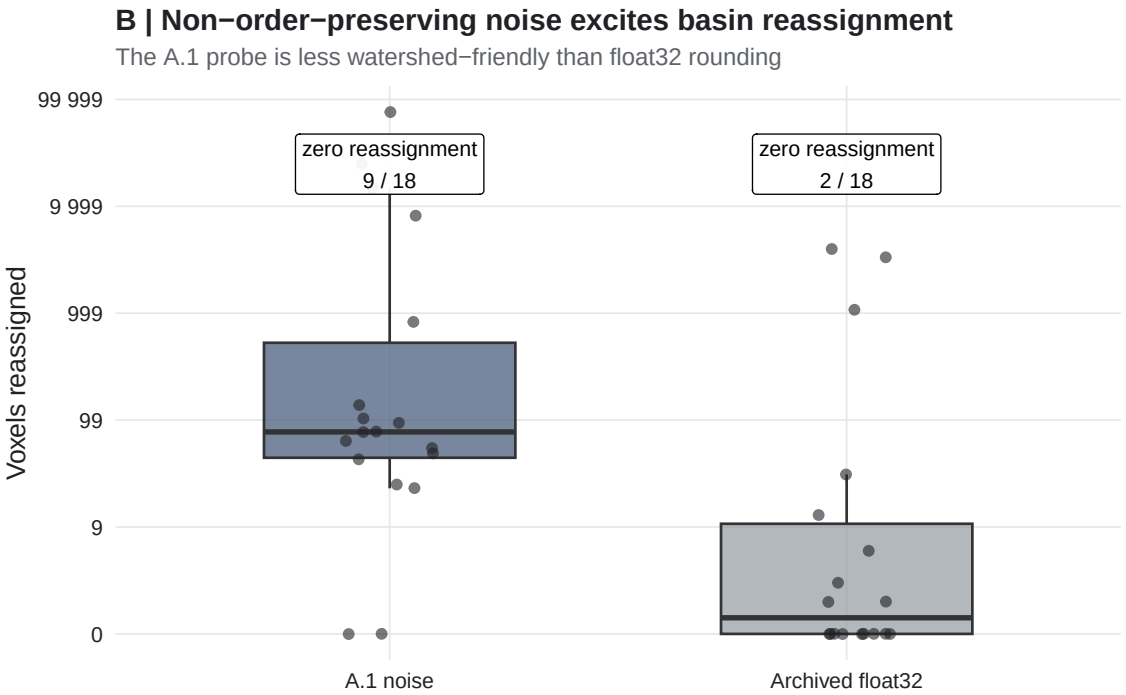


Supplementary Figure S2 | Protocol A.1 probe validation, seed sensitivity and amplitude sensitivity

Five fixed seeds and a maximum-over-seeds floor are used to make numerical eligibility conservative and auditable; the amplitude remains explicitly part of the protocol definition.

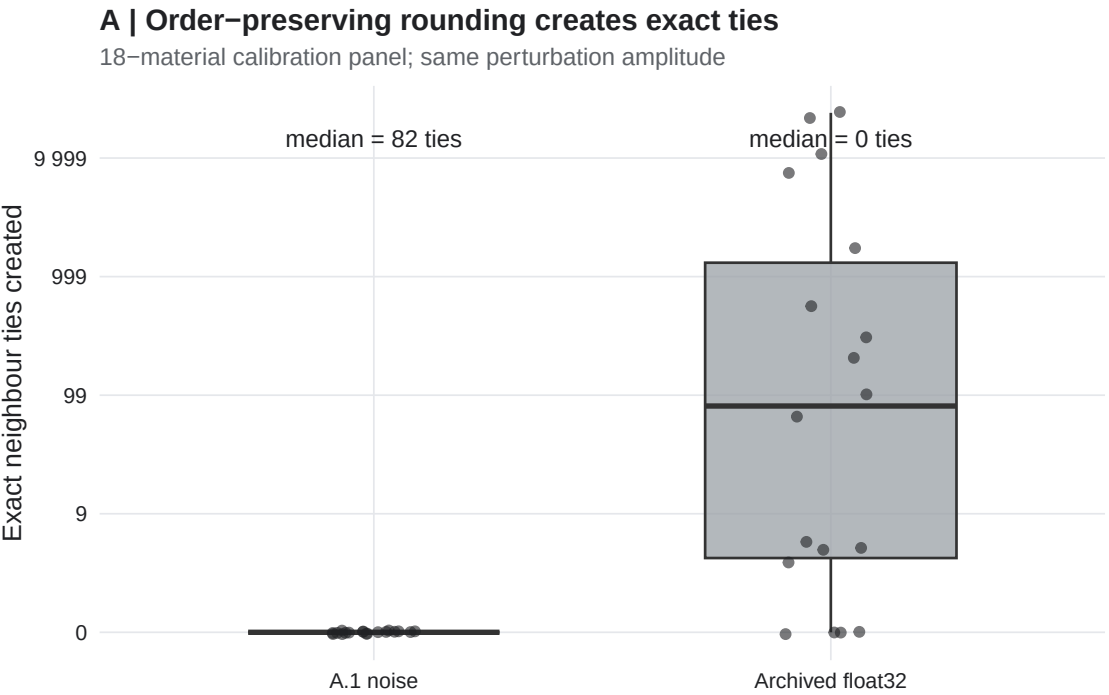

A–B. Eighteen-material pre-freeze calibration comparing archived float32 rounding with uniform noise at the same amplitude. C. Full-corpus five-seed variability and eligibility changes relative to the primary seed alone. D. Two-decade amplitude