IQMS User Letter 51 – PTC handling for Copper Intra-Uterine Device (IUD) medical devices Nova T and Nova T 380

Version: 5.0
Effective Date: 2025-02-24
Applicable to: Nova T and Nova T 380

1. IUD – General Guidance

This User Letter provides guidance on PTC entry for Cooper IUD medical devices. The Copper IUD (Intrauterine Device) products Nova T and Nova T 380 are class III Medical Devices and therefore, all cases require RQU investigation (full workflow for all cases including usability issues and cases where no sample and/or batch are available).

Sample: The root cause cannot be investigated without the sample therefore provision of sample is needed. If the sample is not available e.g. sample cannot be sent, photos shall be provided. In some rare package related issues, photos are sufficient.

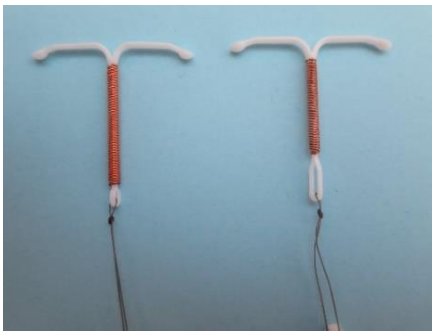
Bayer product: Nova T 380 (left site) and Nova T (right site)	**NovaPlus T 380 manufactured by Eurogine S.L**
	
Nova T & T 380 copper IUDs have brow/gray threads, and the T-body loop is oval eyelet	Nova T is mixed up with Nova Plus T 380 manufactured by Eurogine S.L. Ask for sample or pictures. Competitor Nova Plus T 380 has blue threads and ball shape T-body loop

Table 1 defines Level 1 (object types) and Level 2 (Error codes) and Level 3 (Error (sub) codes), Adverse Event types and risk category for copper IUDs related defects (not all inclusive). In addition, guidance on incident category is including. Please note that guidance on incident category may change based on the specific situations & scenarios.
N

Abbreviations: AE = Adverse Event; IUD = Intra-uterine Device; HCP = Healthcare Professional; LOE = Lack of Effect; PTC = Product Technical Complaint

Note: introduced changes are in blue

Support: Global Complaint Management
PH: Helene Janzen <helene.janzen1@bayer.com>
CH: Sylvie Soret <sylvie.soret@bayer.com>

INTERNAL

Table 1: Complaint Guidance data entry

PRODUCT COMPLAINT REASON	LEVEL 1	LEVEL 2	LEVEL 3	INITIAL RISK CLASS	ADVERSE EVENT TYPE incl. INCIDENT CATEGORY
T-body arms would not retract into tube, not able to load	Copper IUD	Problem loading	T-body arms would not retract into tube	Low	Non serious incident
Releasing problem related to suspected product defect	Copper IUD	Problem releasing	IUD did not release from insertion tube	Low	Non serious incident
T-Body Loop breakage or damage	Copper IUD	Damage to T-body loop	During loading *or* during insertion *or* during use / in situ *or* during removal	Medium	Serious incident
			During loading * *or* Other *	Low	Non serious incident
Breakage or damage to T-body other than loop	Copper IUD	Damage to T-body other than loop	During loading *or* during insertion *or* during use / in situ *or* during removal	Medium	Serious Incident
			During loading * *or* Other *	Low	Non serious incident
T-body arms fail to open in situ	Copper IUD	Damage to T-body other than loop	Arms bent *or* Other	Low	Non serious Incident
Damage to copper wire	Copper IUD	Damage to copper wire	Other	Low* Medium	Serious Incident
Insertion tube bent or otherwise damaged	Copper IUD	Damage to insertion tube	Tube bent *or* Other	Low	Non serious Incident
Thread Breakage or Detachment	Copper IUD	Problem with threads	Threads broke / detached during loading or threads broke / detached during insertion *or* threads broke / detached during use / in situ *or* threads broke / detached during removal	Medium	Serious Incident

INTERNAL

PRODUCT COMPLAINT REASON	LEVEL 1	LEVEL 2	LEVEL 3	INITIAL RISK CLASS	ADVERSE EVENT TYPE incl. INCIDENT CATEGORY
			Threads broke / detached during loading*	Low	Non serious Incident
Issue with threads (no breakage reported)	Copper IUD	Problem with threads	Other	Low	Non serious Incident
Plunger damage	Copper IUD	Damage to plunger	Other	Low	Non serious Incident
Problems with flange	Copper IUD	Problems with flange	Other	Medium	Serious Incident
Flange loose	Copper IUD	Problems with flange	Other	Low	Non serious incident
Received Damaged – blister, Lack of sterility (not used for insertion)	Copper IUD	Received damaged	Sterile packaging, other damages *or* Sterile packaging, seam open	Low	Non serious incident
Received Damaged – blister, Lack of sterility (used for insertion)	Copper IUD	Received damaged	Sterile packaging, other damages *or* Sterile packaging, seam open	Medium	Serious Incident
Received Damaged – folding box (Not attributed to shipping)	Folding box	Damage	Breakage, Open, Originality seal damaged, Originality seal missing, Other	Low	Non serious Incident
Missing batch number or expiration date – folding box	Folding box	Print/Labelling	Variable data missing	Low	Non serious Incident
Missing batch number – blister	Copper IUD	Print/Labelling	Batch missing on sterile packaging	Low	Non serious Incident
Missing leaflet	Folding box	Quantity	Leaflet missing	Low	Non serious Incident
Missing product / component	Copper IUD	Quantity	Component missing, Device missing in sterile packaging	Low	Non serious Incident

INTERNAL

PRODUCT COMPLAINT REASON	LEVEL 1	LEVEL 2	LEVEL 3	INITIAL RISK CLASS	ADVERSE EVENT TYPE incl. INCIDENT CATEGORY
Adverse reaction (Incident)	---	----	---	Low	Non serious Incident Expulsion or Dislocation or Spasm or Removal or procedural pain and bleeding or increased bleeding /menstruation or other
Adverse reaction (Incident)	---	---	---	Medium	Serious Incident Dislocation** *or* Removal** *or* other**
Adverse reaction (Incident) e.g. perforation or embedment	---	---	---	Medium	Serious Incident Perforation or removal**
LOE (Lack of effect)	---	---	---	Medium	Serious Incident Pregnancy incl. ectopic pregnancy
Usability issues related to use error	Copper IUD	Use error	Instructions not followed *or* failed insertion *or* incorrect insertion technique *or* Came out with scissors or speculum *or* Insertion tube bent *or* Difficulty cutting threads *or* Excess force used	Low	Non serious Incident
Customer satisfaction issues (no use error)	Copper IUD	Customer Satisfaction Issue	Anatomical reasons *or* Expelled in the office *or* Opening of the package difficult *or* contaminated prior use by user *or* Other	Low	Non serious Incident
Medication error e.g. used after expiry date	---	---	used after expiry date *or* used for wrong indication *or* used for too long time (available) *or* other	Low	Non serious Incident
Contamination inside the package or in product e.g. particle inside blister.	Copper IUD	Contamination/Foreign matter	Contamination or foreign material in package / device	Low	Non serious Incident

INTERNAL

PRODUCT COMPLAINT REASON	LEVEL 1	LEVEL 2	LEVEL 3	INITIAL RISK CLASS	ADVERSE EVENT TYPE incl. INCIDENT CATEGORY
(not used for insertion)					
Contamination inside the package or in product e.g. particle inside blister. (used for insertion)	Copper IUD	Contamination / Foreign material	Contamination or foreign material in package / device	Medium	Serious Incident

*Noted before insertion, patient not involved

** With surgical intervention (Add “serious incident” as Adverse Event Type)

Reportable cases (Serious incidents)
Device breakage
Device related sepsis
Ectopic pregnancy with contraceptive device
Embedded device
Pregnancy with contraceptive device

INTERNAL