
IQMS User Letter 72 – Change of Complaint Process for Betaconnect

Version: 1.0
Effective Date: 2026-01-01
Applicable to: GBS/CQU

Dear CQU and GBS Users,
This user letter guides the complaint processing for Betaconnect (Autoinjector for Betaferon) manufactured by an external Legal Manufacturer (LM) Phillips-Medisize A/S (Struer) with Bayer as distributor.

Guidance for PTC or PTC+AE Entry in IQMS

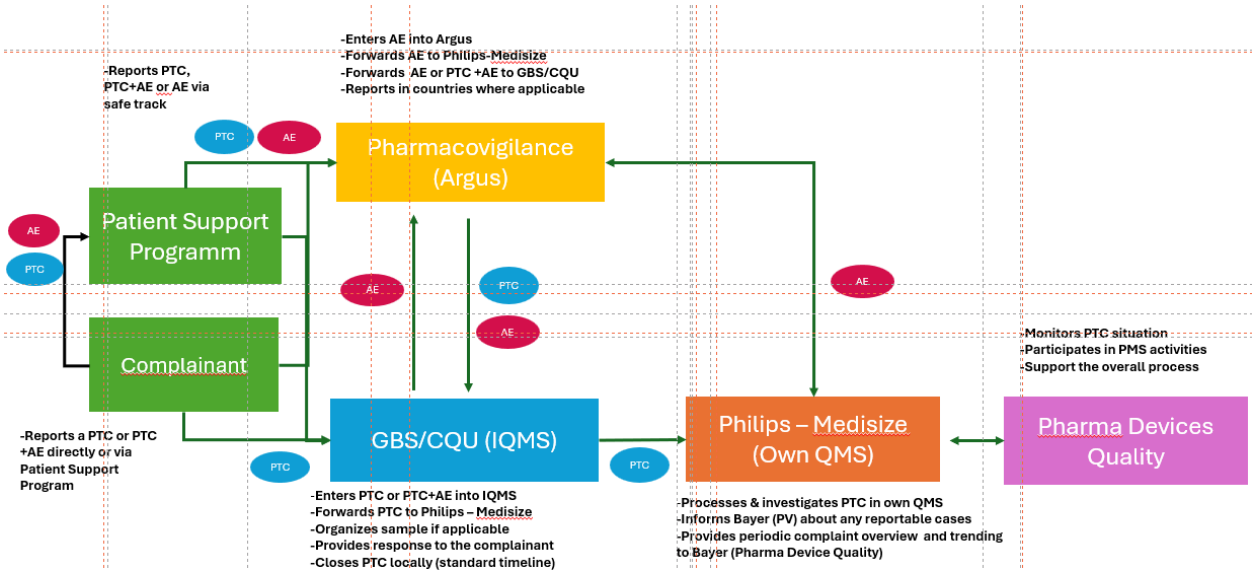

Scenario 1: PTC or PTC+AE is forwarded by complainant / PSP directly to quality:

1. Enter PTC or PTC+AE in IQMS.
2. Forward the complaint including the formatted output to the Legal Manufacturer via email. Acknowledgement: The LM will acknowledge receipt of the complaint via email.
3. If LM requires additional information: obtain further information from complainant and forward it to the LM (email).
4. Organize sample retrieval shipment as applicable.
5. If a response letter is requested: Provide a standard response letter. In individual cases request support from Medical Device Quality: “MedicalDevice.Complaints" medicaldevice.complaints@bayer.com. Medical device quality will ad hoc clarify with legal manufacturer the content.
6. PTC only: lose Case locally (standard timeline).

Note: PTC is associated with and AE: Forward to PV, await and reference Global Database Safety Number in IQMS and close the case locally (standard timeline).
Note: Upon PTC investigation receipt, CM PQS Rep is responsible for entering the PTC investigation result directly in the Global Safety Database.

INTERNAL

Scenario 2: PTC or PTC+AE is forwarded by PV to Quality:

- Process PTC or PTC+AE as per scenario 1 (step 1-5).
- Close PTC+AE locally (no need to forward for investigation / start QSE).
  Note: The legal manufacturer will forward investigation results to Bayer PV e.g. MIR if applicable.

IQMS Field	Content
Division	Pharma
Product Type	RoW: Medical Device; US: Combination Product
Feedback type	Documentation
Batch / Serial Number Status	N/A or Yes (if batch is available) If serial number is available, include serial number of the injector in the "Description" field.
Batches Section	If batch number is available add the batch number in the "batches" section. Note: Batch number is only available on the co-packaged pack but not on the injector.
Adverse Event Reported is "Yes"	Reference Global safety Database Number
Legal Manufacturer	Phillips-Medisize A/S (Struer)
Owning Organization	Country Organization e.g. CO USA (US03)
Local Closure?	Yes
Rationale for Local Closure	Legal Manufacturer Informed
Impacted Organization	Phillips-Medisize A/S (Struer)
Error codes, Initial Risk Class	Based on complaint description

Expired Devices:
Expired devices **with and without PTC** can be disposed of (exception: AE-related)
CQU should send a quarterly list of expired devices which have been disposed of to the Legal Manufacturer (documentation to be stored locally).

LM email contact details, email address (Complaint / follow-up information)	LM Sample Shipping address
complbayerbetaconnect@molex.com	Phillips-Medisize A/S (Struer) c/o Khalid Chajia Gimsinglundvej 20, DK-7600 Struer, Denmark

Abbreviations: AE=Adverse event, CQU=Country Quality Unit, GBS=Global Business Services (GBS), LM=Legal Manufacturer PTC= Product Technical Complaint

This user letter remains valid until further notice.

Support: Global Complaint Management: Helene Janzen <helene.janzen1@bayer.com

INTERNAL