INSPIRE - 100

An Emergency Ventilator

TekMedika Pvt. Ltd.

INSPIRE-100 is a patent-pending ventilator design tailored for adult patients, providing comprehensive ventilatory support from initiation to weaning.

It features a user-friendly Human-Machine Interface with a clear front panel and advanced remote monitoring capabilities accessible via laptops, desktops, tablets, or mobile devices.

This device is particularly suited for facilities without access to compressed gas or oxygen pipelines and is built to withstand challenging environmental conditions.

INSPIRE-100 supports four commonly used ventilation modes: CMV, ACV, SIMV, and PSV. It offers a full range of breath parameters across all modes, ensuring complete assistance for patient-initiated breathing.

- ✓ Unmatched Affordability
- ✓ Unmatched Remote Monitoring via WiFi
- ✓ Unmatched Ease-of-use
- ✓ Works without Compressed Air Pipeline
- ✓ Works with Oxygen Cylinder or Concentrator
- ✓ Field Upgradeable
- ✓ Complete Set of mainstream Parameters

Intended Use

Adult Patients only

✅ Acute Respiratory Distress Syndrome (ARDS)

✅ Chronic Obstructive Pulmonary Disease (COPD)

✅ Obese Hypoventilation Symptoms (OHS)

✅ Cheyne-Stokes breathing (CSR/CSA)

✅ Neuromuscular Diseases

✅ Pneumonia

✅ Asthma

✅ Drug Overdose

✅ Snake Bites

Technical Specs

Mode	Description
CMV	Continuous Mandatory
ACV	Synchronized Assist Control
SIMV	Synchronized Intermittent Mandatory
PSV (BiPAP)	Pressure Supported (BiPAP equivalent)

Volume Control Parameter	Range
Tidal Volume (ml)	200 - 600
Respiration Rate (bpm)	10 - 30
I:E Ratio	1:1 - 1:3
PEEP (cmH2O)	4 - 15
FiO2 (System Managed)	External

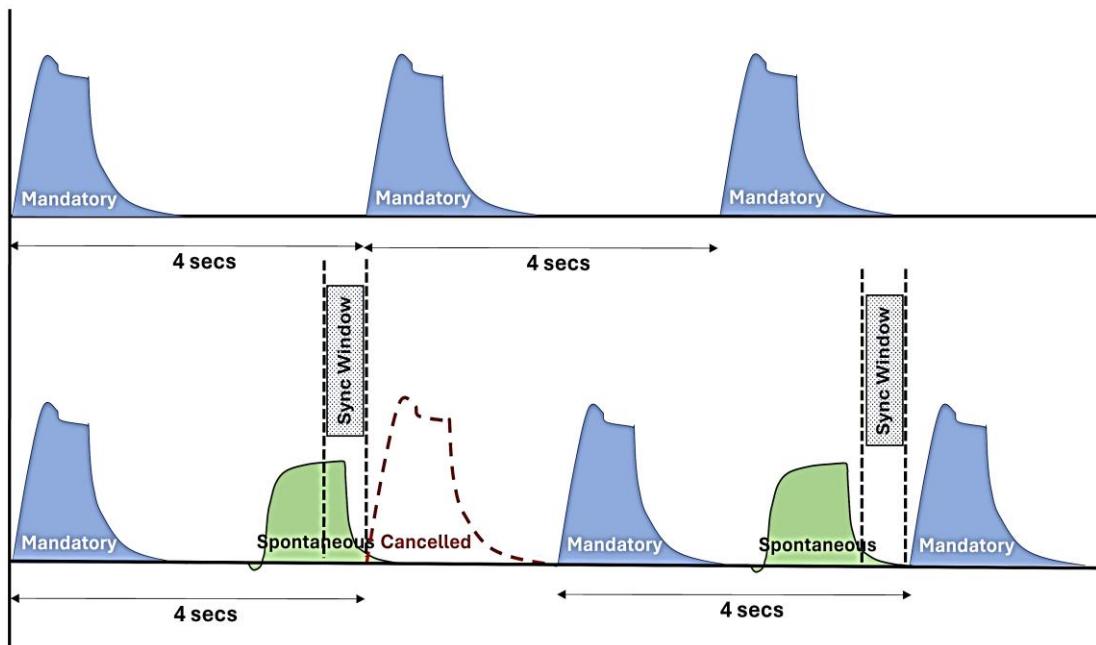| Pressure Support Parameter	Range
Support Pressure (cmH2O)	5 - 20
Flow Trigger Termination (%)	10 - 60

Full Set of ALARMS	
Max Pressure	Pressure Leak
Pressure Loss	Airway Blockage
Cough / Hiccups	System Temperature
Inconsistent Parameters	Extreme Parameters
Replace BVM	BVM Size
and many more ...	

Power Consumption 120W
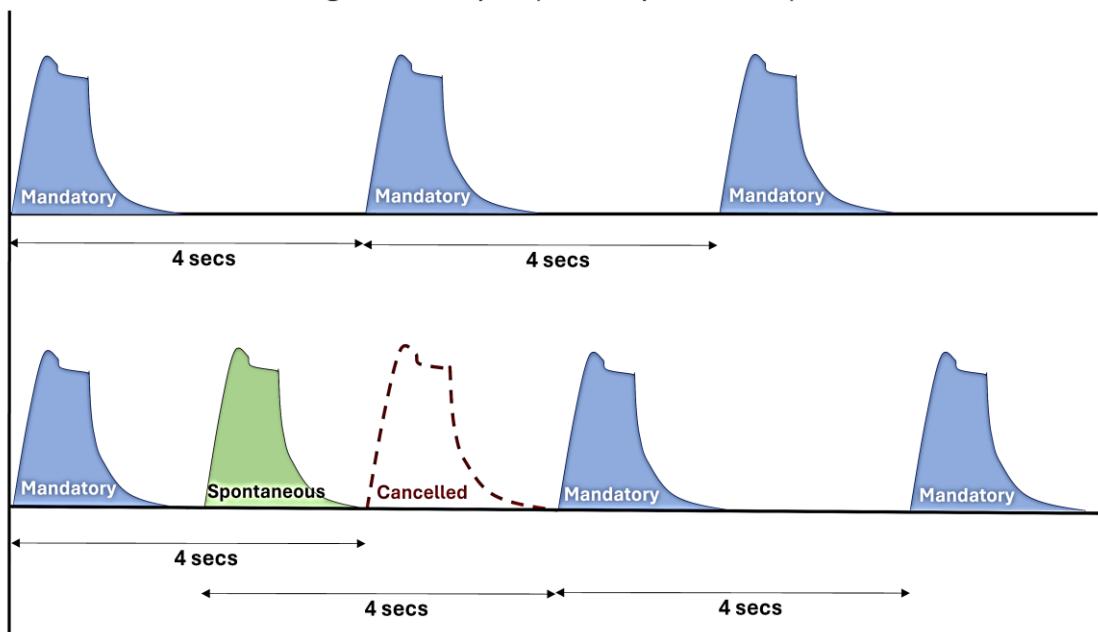
Breath Synchronization for Patient Comfort

Breath Synchronization in SIMV Mode
e.g. RR=15 bpm (4 secs per breath)

Mandatory · Mandatory · Mandatory · 4 secs · 4 secs · Sync Window · Mandatory · Spontaneous · Cancelled · Mandatory · Spontaneous · Mandatory · Sync Window · 4 secs · 4 secs
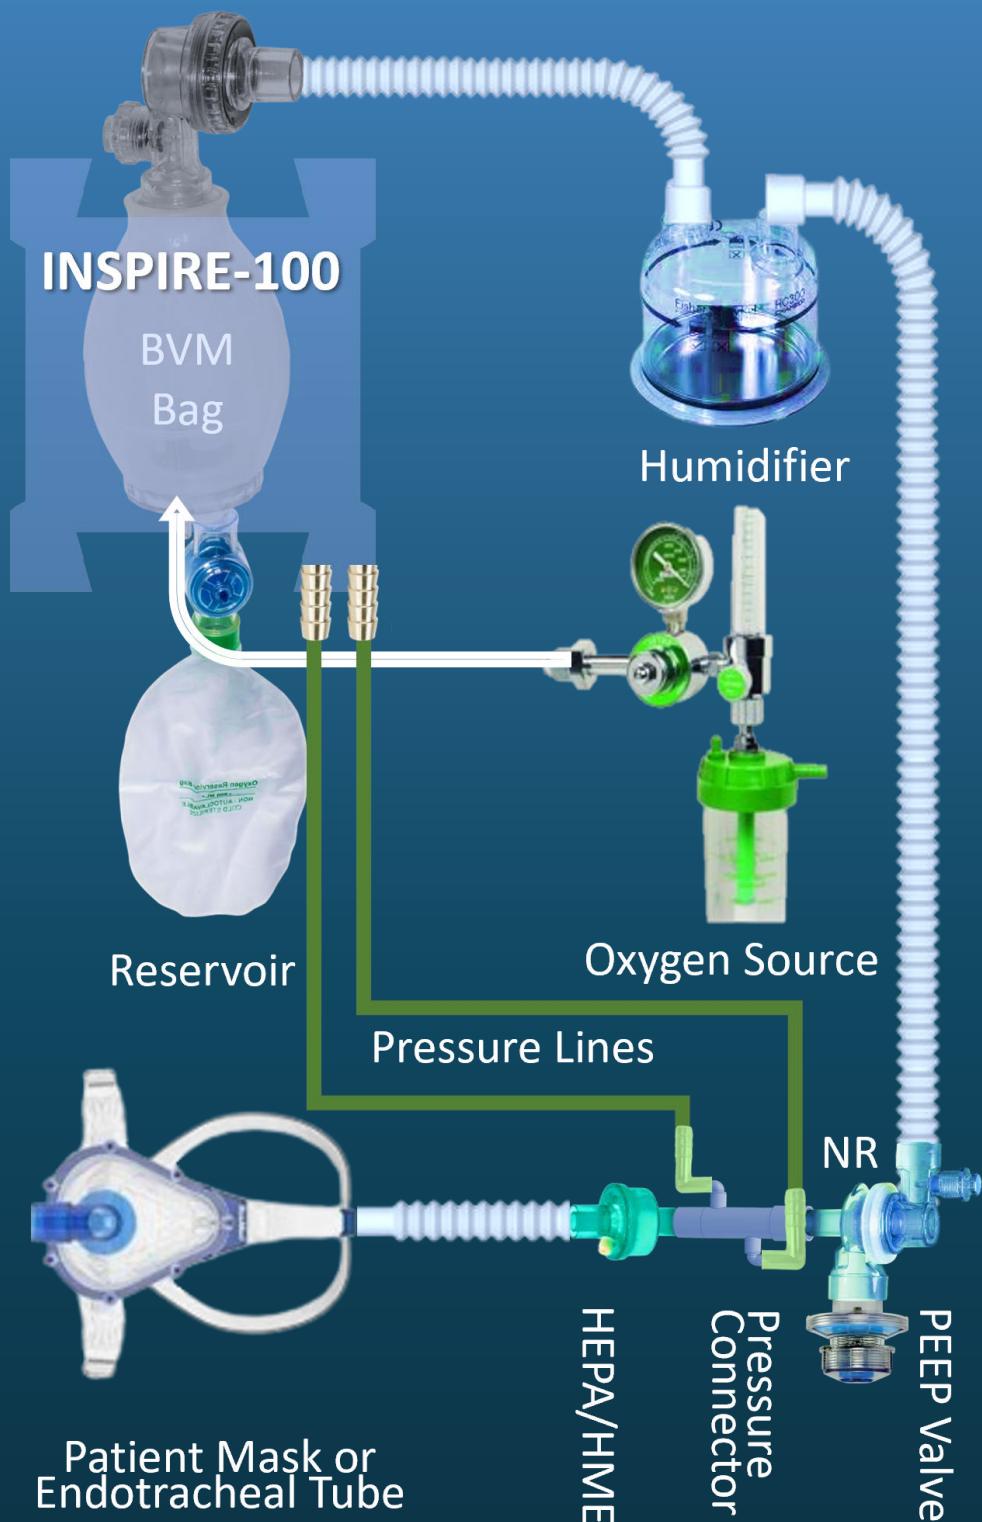
Breath Synchronization in ACV Mode
e.g. RR=15 bpm (4 secs per breath)

Mandatory · Mandatory · Mandatory · 4 secs · 4 secs · Mandatory · Spontaneous · Cancelled · Mandatory · Mandatory · 4 secs · 4 secs · 4 secs
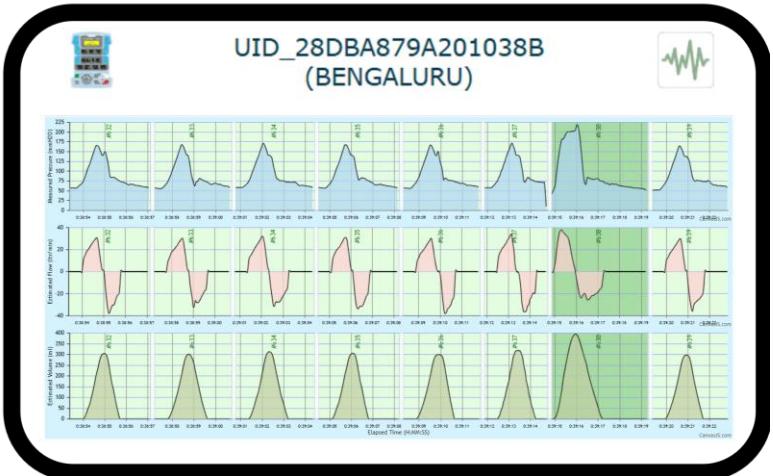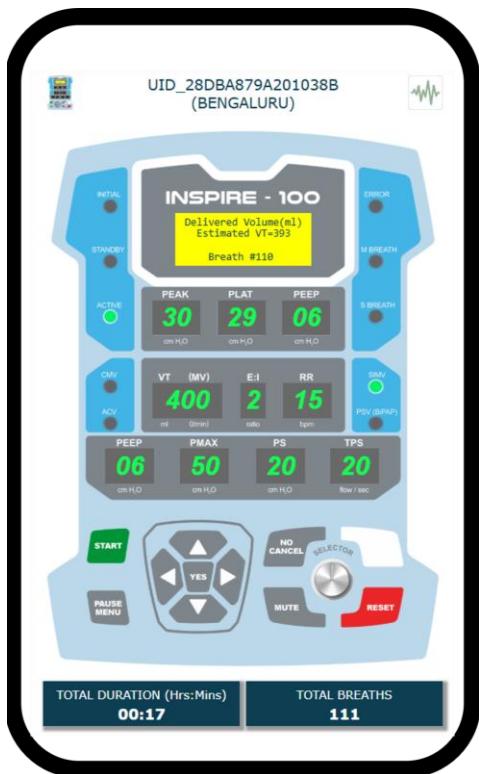
Breathing Circuit

Simple, Off-the shelf, Single-limbed and compatible with Standard Accessories

INSPIRE-100

BVM Bag

Humidifier

Reservoir

Oxygen Source

Pressure Lines

NR

Patient Mask or Endotracheal Tube

HEPA/HME

Pressure Connector

PEEP Valve

Remote Monitoring

- ✓ Accessible on Laptops & Mobile devices
- ✓ Search & Range Selection
- ✓ Snapshots View
- ✓ Waveforms View
- ✓ Charts View
- ✓ Statistics View
- ✓ Recording and Playback
- ✓ Multi-system Display

Powerful Search for Combination of Events

Demo Long [09-05-2024 17:40:26]

MATCH CRITERIA

((MODE_SETTING == "SIMV") AND ((BREATH_TYPE == "MANDATORY") AND ((TIDAL_VOLUME < 250) OR (PEAK_PRESSURE > 30))))

MODE_SETTING	EQ	SIMV	
AND			
BREATH_TYPE	EQ	MANDATORY	
AND			
TIDAL_VOLUME	LT	250	ml
OR			
PEAK_PRESSURE	GT	30	cmH2O

CLEAR   EXPORT   IMPORT   SEARCH

SEARCH RESULTS in Breath number range [1, 128]
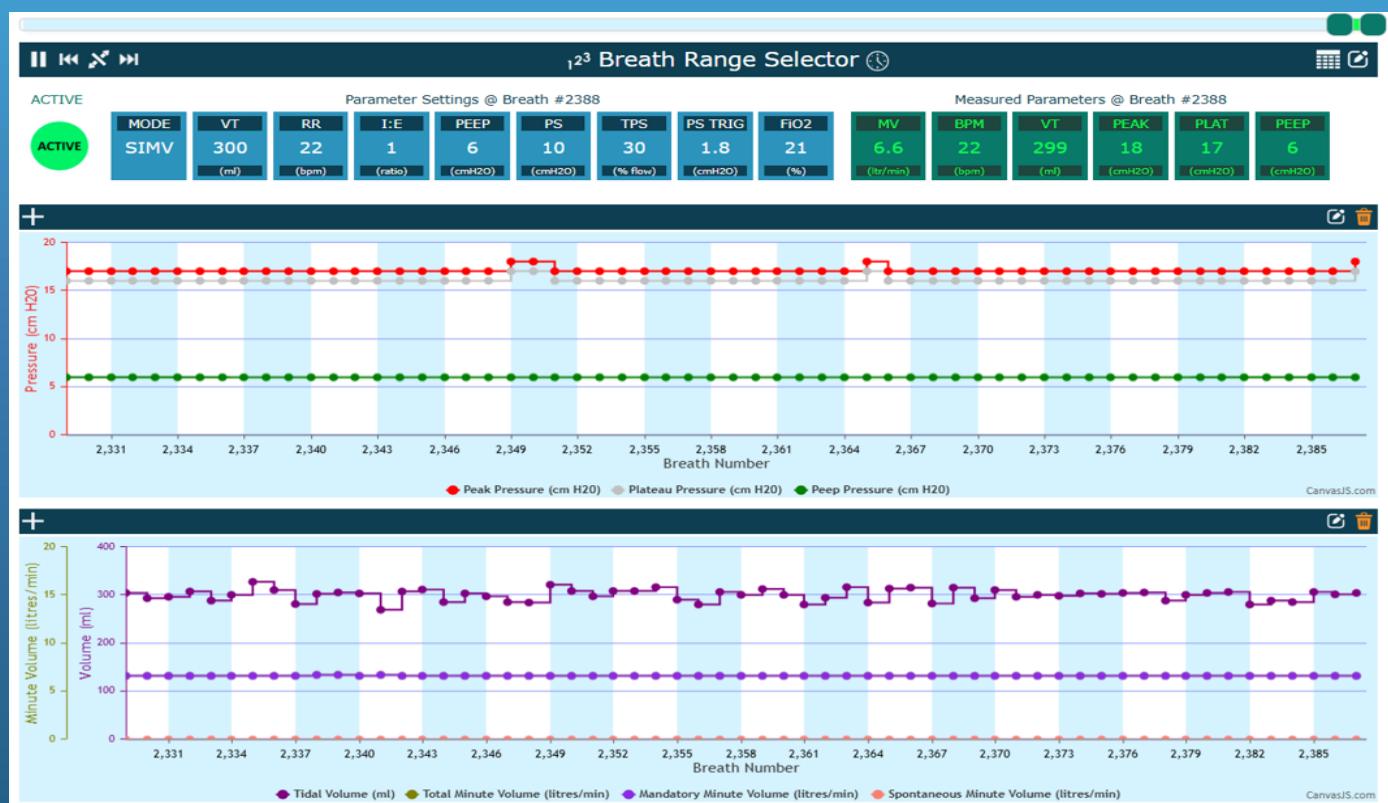
Range	Matching Breaths			Parameter Values			
Select	Number	Date	Time	MODE_SETTING	BREATH_TYPE	TIDAL_VOLUME	PEAK_PRESSURE
☐	9	09-05-2024	17:40:56	SIMV	MANDATORY	229	37
☐	10	09-05-2024	17:41:00	SIMV	MANDATORY	252	34
☐	11	09-05-2024	17:41:04	SIMV	MANDATORY	278	36
☐	43	09-05-2024	17:43:31	SIMV	MANDATORY	216	10
☐	44	09-05-2024	17:43:35	SIMV	MANDATORY	216	10
☐	46	09-05-2024	17:43:43	SIMV	MANDATORY	205	22
☐	47	09-05-2024	17:43:47	SIMV	MANDATORY	227	24
☐	48	09-05-2024	17:43:51	SIMV	MANDATORY	234	23
8 Matches: End of Search							

Range Selector to Navigate Any View Back and Forth in Time
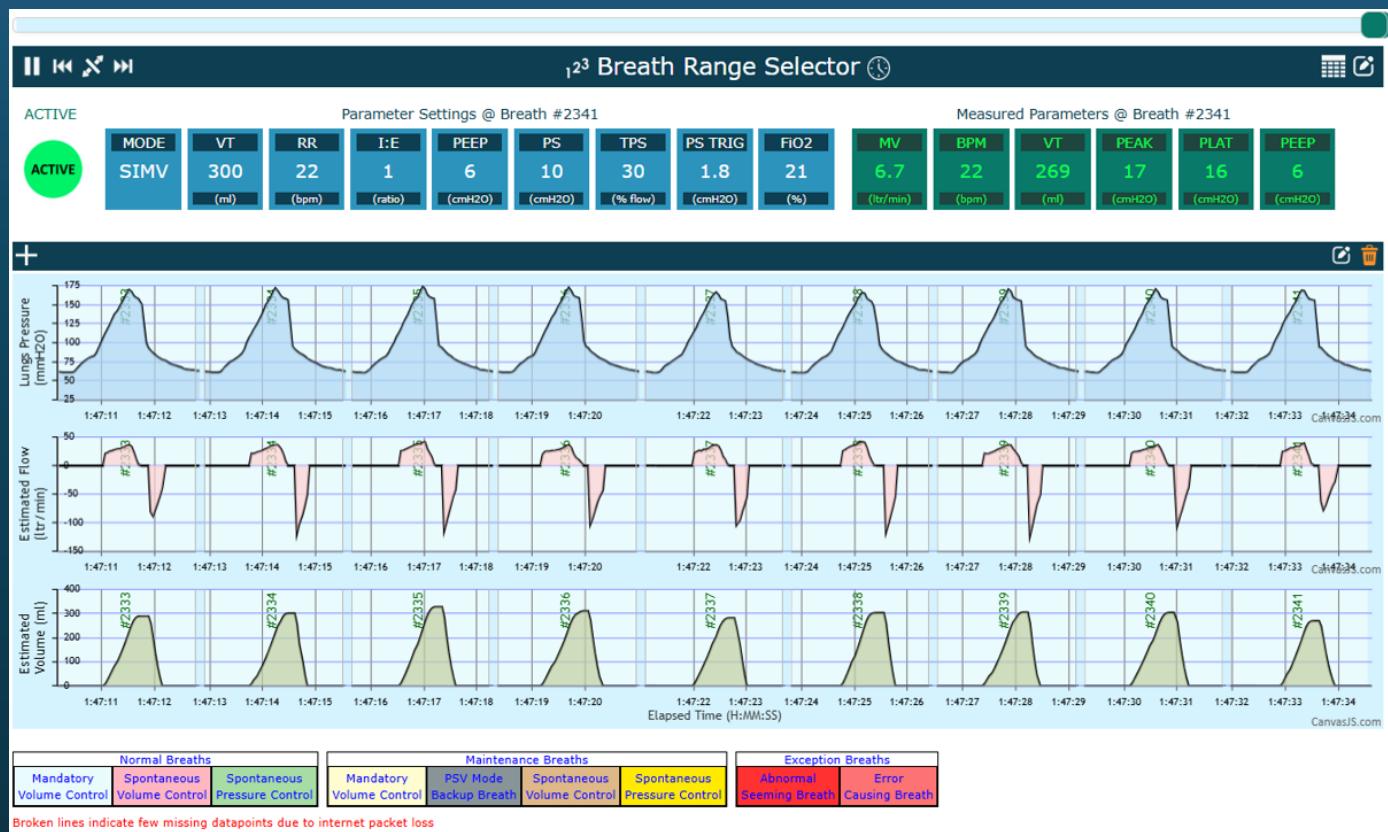
123 Breath Range Selector

Selected Breath Range

	Breath Number	Breath Start Time		
		Day	Date	Time
From	520	Fri	26-Apr-2024	12:20:05
Upto	579	Fri	26-Apr-2024	12:22:58
SPAN	60		00:02:53	
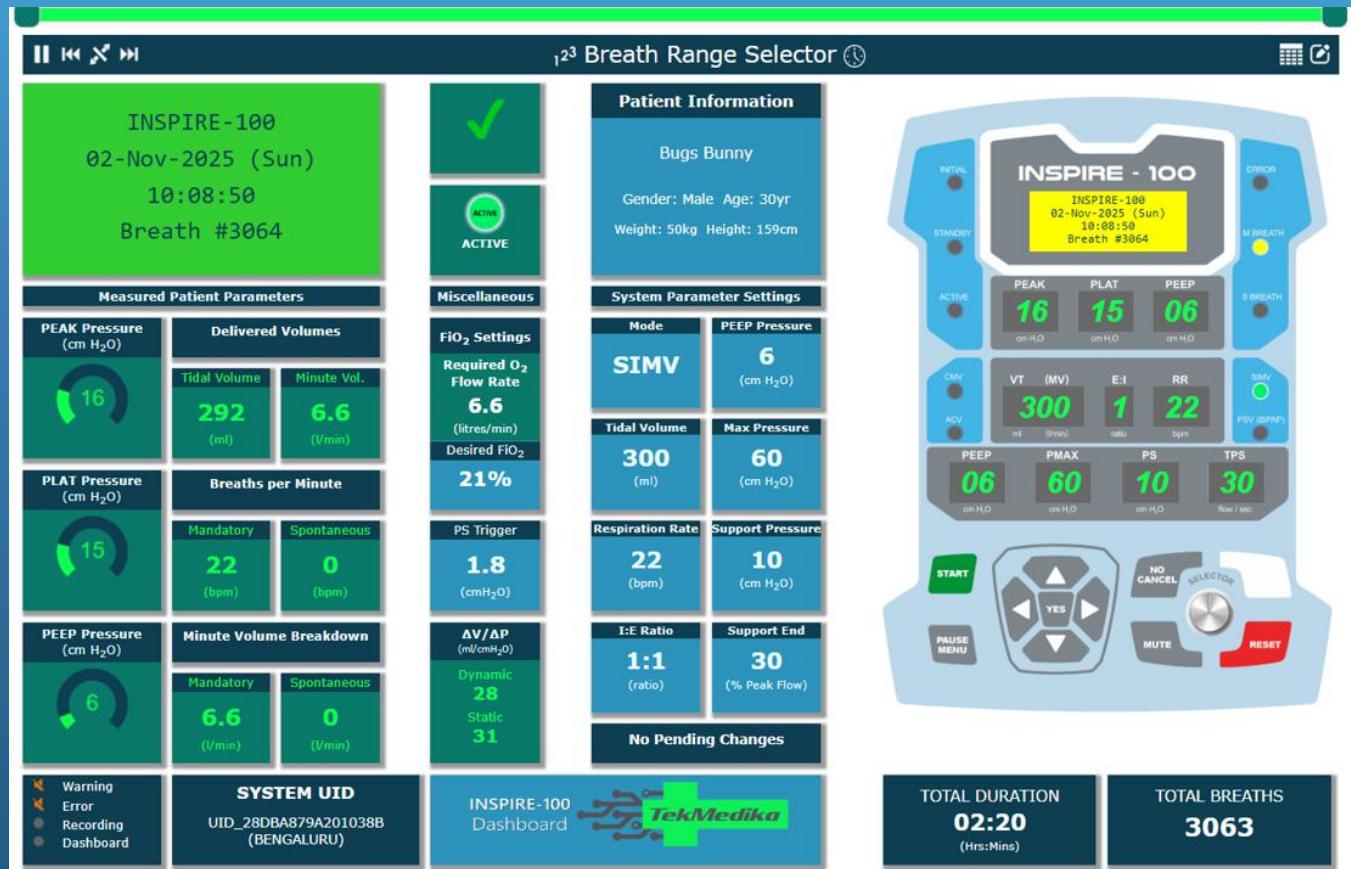
Charts for All Parameters

Pressure & Flow Waveforms

Snapshots for each Breath

INSPIRE-100
02-Nov-2025 (Sun)
10:08:50
Breath #3064

✓

ACTIVE

Measured Patient Parameters

PEAK Pressure (cm H2O): 16

Delivered Volumes
Tidal Volume	Minute Vol.
292 (ml)	6.6 (l/min)

PLAT Pressure (cm H2O): 15

Breaths per Minute
Mandatory	Spontaneous
22 (bpm)	0 (bpm)

PEEP Pressure (cm H2O): 6

Minute Volume Breakdown
Mandatory	Spontaneous
6.6 (l/min)	0 (l/min)

Warning
Error
Recording
Dashboard

SYSTEM UID
UID_28DBA879A201038B
(BENGALURU)

INSPIRE-100 Dashboard TekMedika

Miscellaneous

FiO2 Settings
Required O2 Flow Rate
6.6 (litres/min)
Desired FiO2
21%

PS Trigger
1.8 (cmH2O)

ΔV/ΔP (ml/cmH2O)
Dynamic 28
Static 31

Patient Information

Bugs Bunny

Gender: Male Age: 30yr
Weight: 50kg Height: 159cm

System Parameter Settings

Mode	PEEP Pressure
SIMV	6 (cm H2O)

Tidal Volume	Max Pressure
300 (ml)	60 (cm H2O)

Respiration Rate	Support Pressure
22 (bpm)	10 (cm H2O)

I:E Ratio	Support End
1:1 (ratio)	30 (% Peak Flow)

No Pending Changes

TOTAL DURATION
02:20 (Hrs:Mins)

TOTAL BREATHS
3063

Detailed Statistics

Parameters Measured

Parameter	Units	Min	Max	Avg
Peak Pressure	cmH2O	21	26	25.7
Plateau Pressure	cmH2O	19	24	23.7
PEEP Pressure	cmH2O	3	6	5.0
Tidal Volume Delivered	ml	284	966	311.9
Total Minute Volume	litres/min	0	5.8	4.3
Mandatory Minute Volume	litres/min	0	4.6	4.1
Spontaneous Minute Volume	litres/min	0	1.9	0.2
Mandatory BPM	bpm	0	15	13.8
Spontaneous BPM	bpm	0	2	0.2
FIO2	%	35	35	35.0
Static ΔV/ΔP	ml/cmH2O	0	18	15.9
Dynamic ΔV/ΔP	ml/cmH2O	0	16	14.4
System Temperature	degC	35	35	35.0
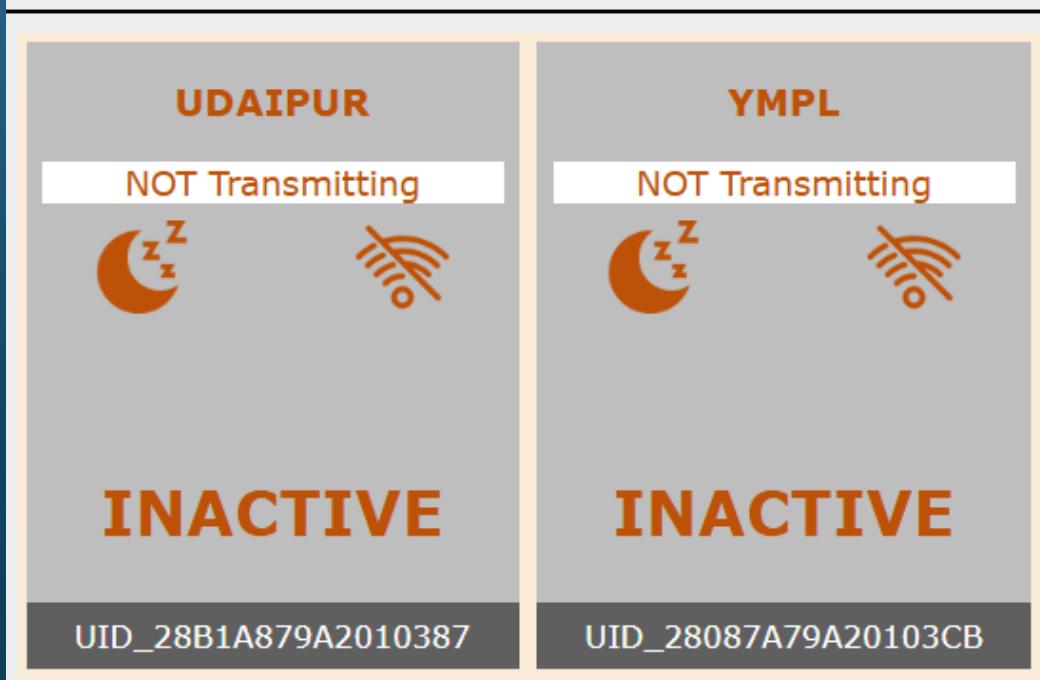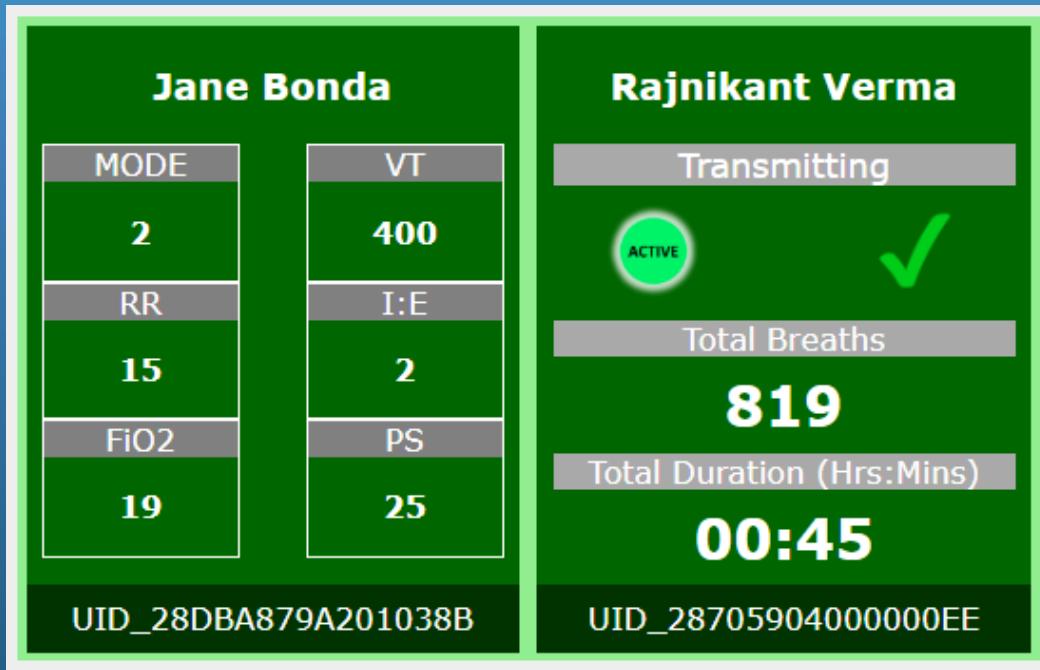
Miscellaneous Information

Information	Value
Number of Breaths	120
Number of Mandatory Breaths	118
Number of Spontaneous Breaths	2
Number of Maintenance Breaths	0
Number of CMV Spontaneous Breaths	0
Number of Missing Intervals (Packet loss)	0
Number of WiFi Disconnects	0
Number of Notifications	0
Number of Warnings	0
Number of Errors	0

Static Information

Patient Name: James Bond007
Gender: Male Age: 42yr
Weight: 76kg Height: 185cm

System Location: Bengaluru
Location Altitude: 3000 ft
Location Atmospheric Pressure: 930 cmH2O
Location Atmospheric Oxygen: 19%

Parameter Settings Used

Parameter	Units	Values
Ventilation Mode	mode	SIMV
Tidal Volume	ml	300
Minute Volume	l/min	2
Respiration Rate	bpm	15
I:E Ratio	ratio	1:2
PEEP Pressure	cmH2O	5
Maximum Pressure	cmH2O	85
Support Pressure	cmH2O	20
Support Pressure Termination	%flow,secs	1.5
FIO2	%	35

Sequence of Parameter Combinations

MODE	VT/MV	RR	I:E	PEEP	PMAX	PS	TPS	FIO2	#BREATHS	Before#
SIMV	300	15	1:2	5	85	20	1.5	35	119	2

Multi-system Monitoring For Nurses Station

Jane Bonda	
MODE	VT
2	400
RR	I:E
15	2
FiO2	PS
19	25
UID_28DBA879A201038B	

Rajnikant Verma

Transmitting

ACTIVE ✓

Total Breaths
819

Total Duration (Hrs:Mins)
00:45

UID_28705904000000EE

UDAIPUR

NOT Transmitting

INACTIVE

UID_28B1A879A2010387

YMPL

NOT Transmitting

INACTIVE

UID_28087A79A20103CB

A summary state of all systems can be displayed on one screen. Each system is shown as a tile.

Proudly Designed & Made in India