



Response to the surface moving — force (top), robot travel (bottom)

syringe in

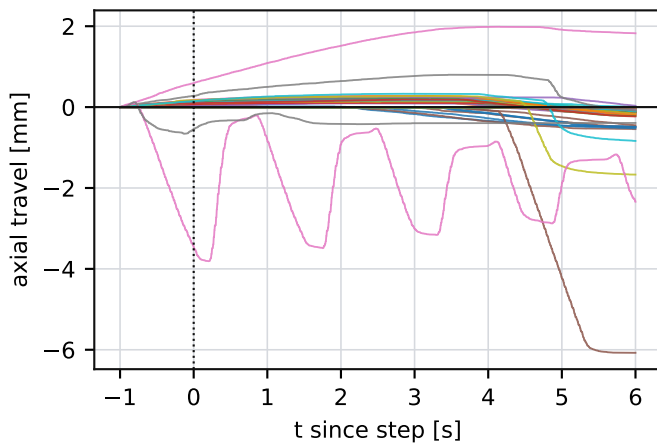

syringe withdraw

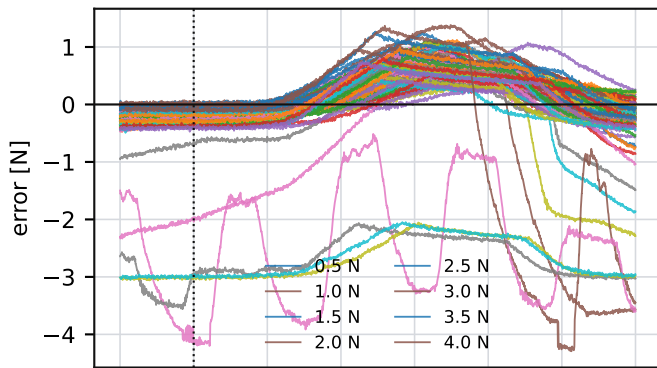