MODEL:

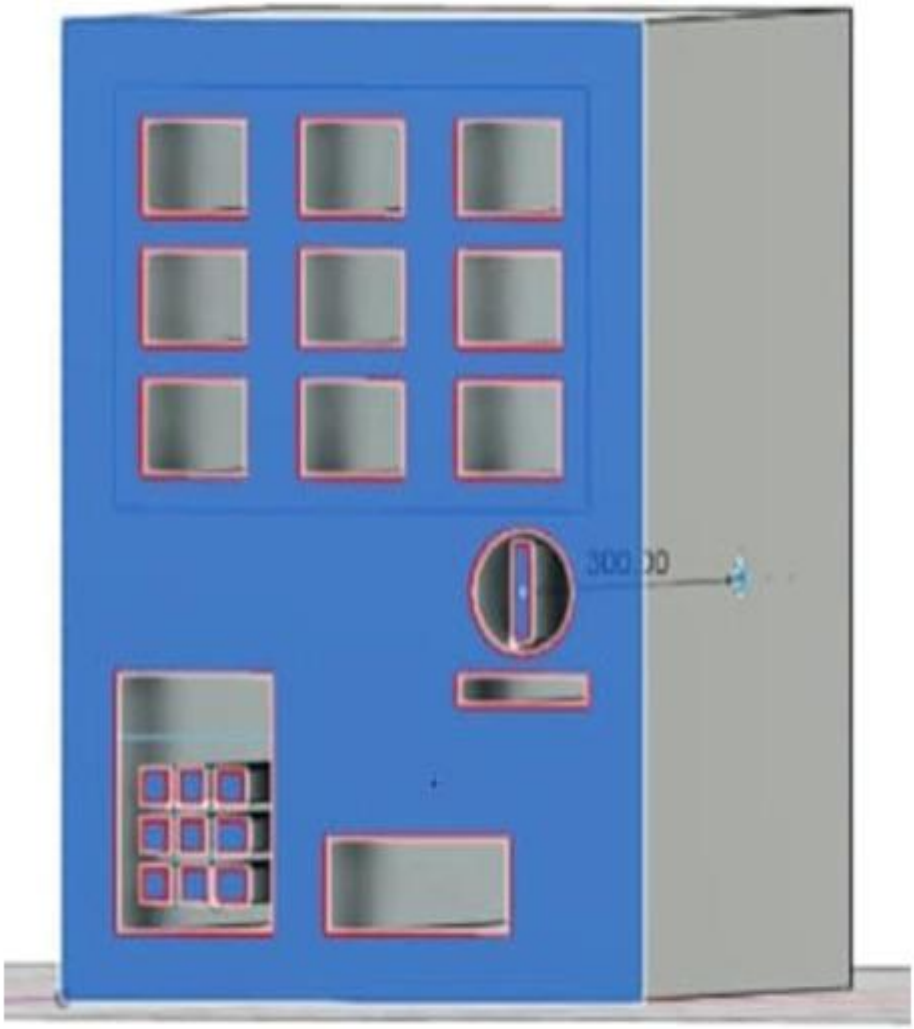

FLOW CHART:

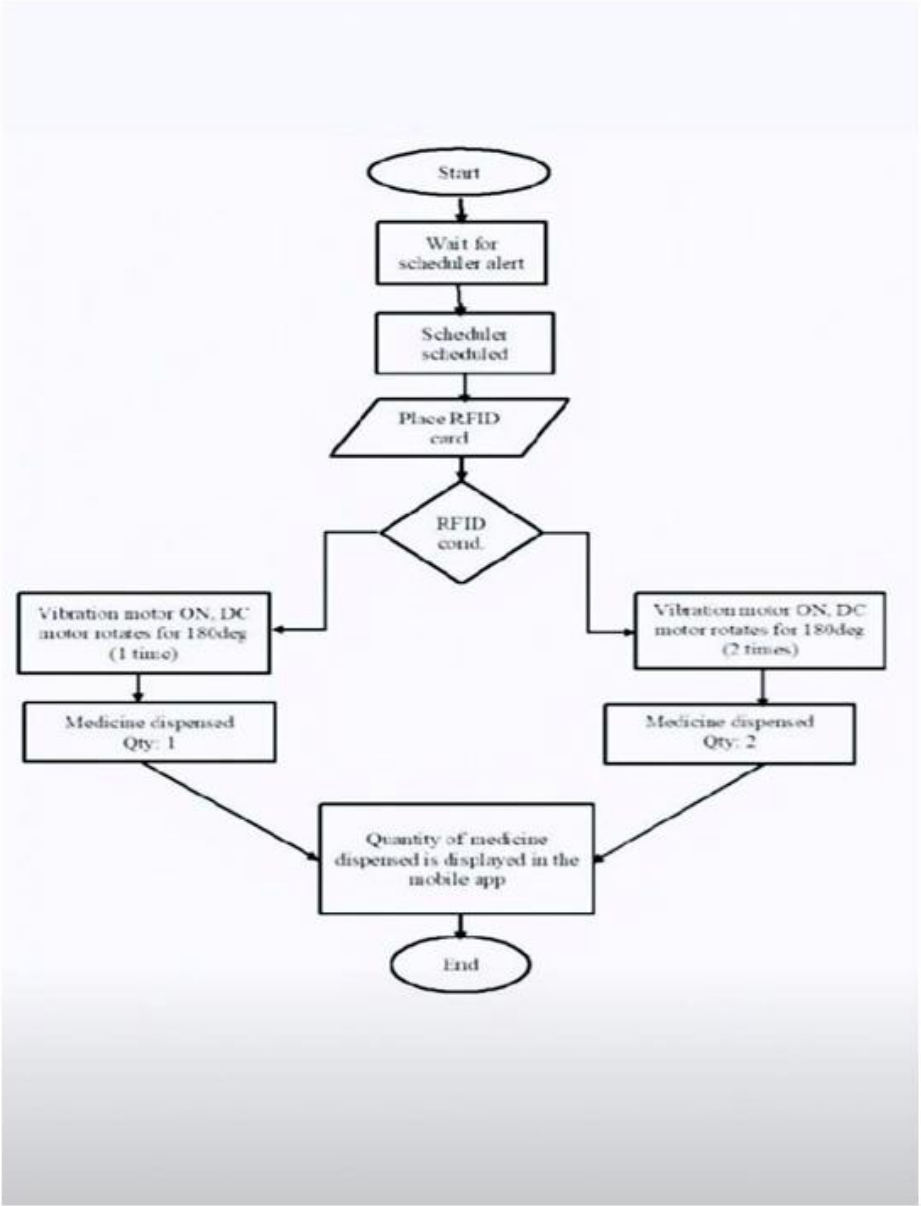
Start
Wait for scheduler alert
Scheduler scheduled
Place RFID card
RFID cond.
Vibration motor ON, DC motor rotates for 180deg (1 time)
Vibration motor ON, DC motor rotates for 180deg (2 times)
Medicine dispensed Qty: 1
Medicine dispensed Qty: 2
Quantity of medicine dispensed is displayed in the mobile app
End
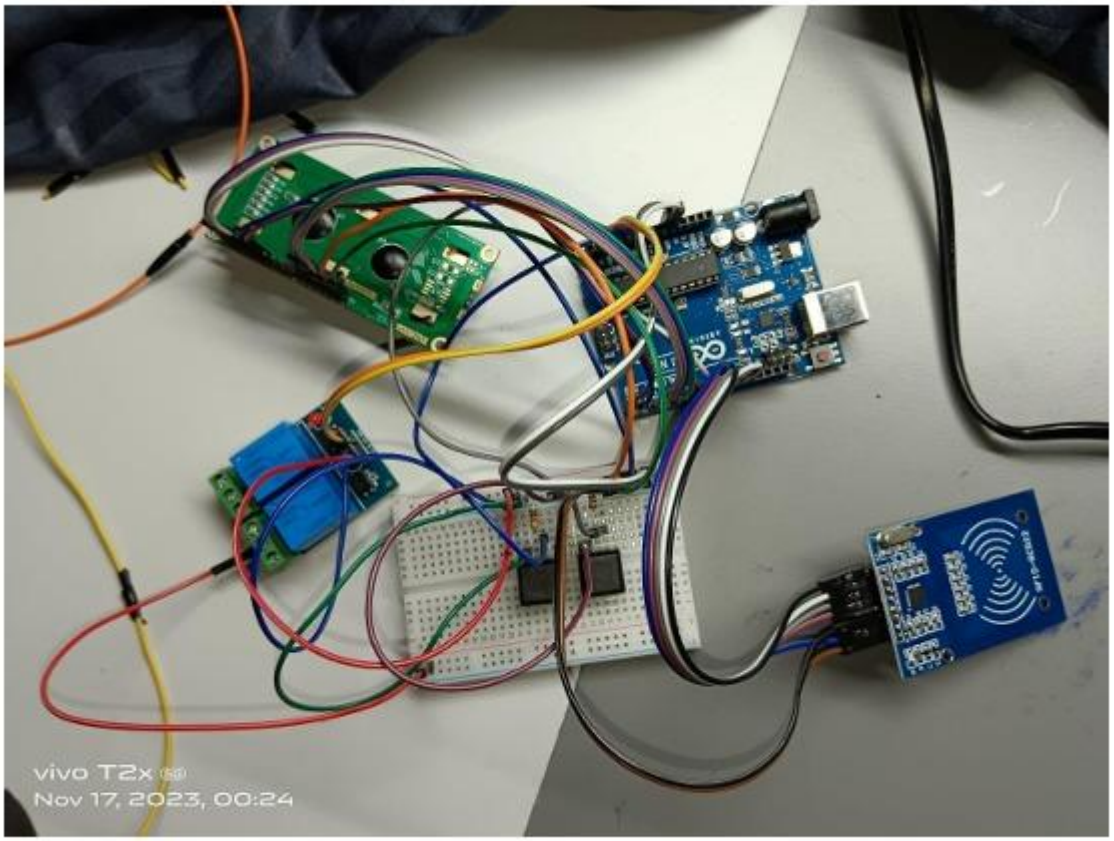
CONNECTION DIAGRAM: