

Polar ECG Analysis Report



Date: 01-01-2026 14:49:46

Elapsed Time: 02:45:58

meanHR	84 [35-200] bpm
HRV	54 [45-67] ms
pNN50	16 [0-55] %
pNN200	1 [0-15] %
meanQRS	67 [50-120] ms
meanQTc	386 [310-470] ms
meanTPositive	99 [90-100] %
meanJPoint	82 [0-500] uV
meanHF	44 [0-90] %
meanSystole	340 [60-2.6k] uV

Beats

13852	Number of beats
17	Number of ectopic beats/events
0.12 %	Percent of ectopic beats/events
1.00 %	Artifact or noise


Heart Rate

120 bpm	Maximum at 15:01:06
52 bpm	Minimum at 14:58:48
99 bpm	Highest 1-minute mean at 14:58:48
72 bpm	Lowest 1-minute mean at 16:02:10
0.00 %	beats in tachycardia (>150 bpm)
0.00 %	beats in bradycardia (<50 bpm)


Rhythm

0	pNN50 episodes
---	----------------


Signal sample

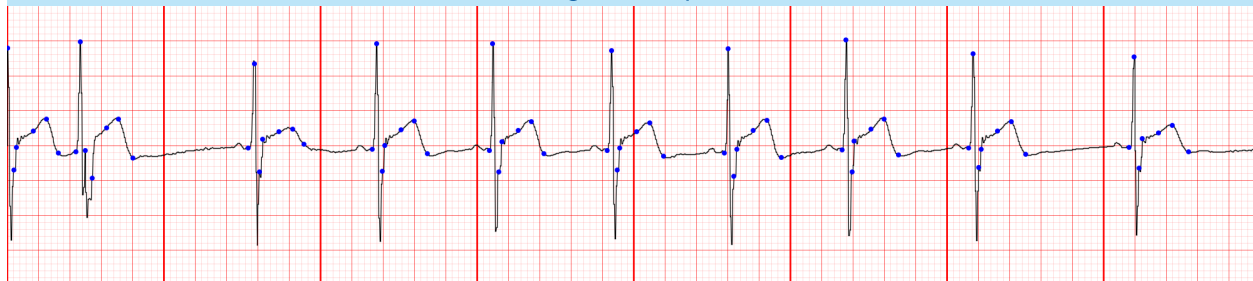


Highest 1-minute meanHR: 99 bpm
(14:57:48 – 14:58:48)

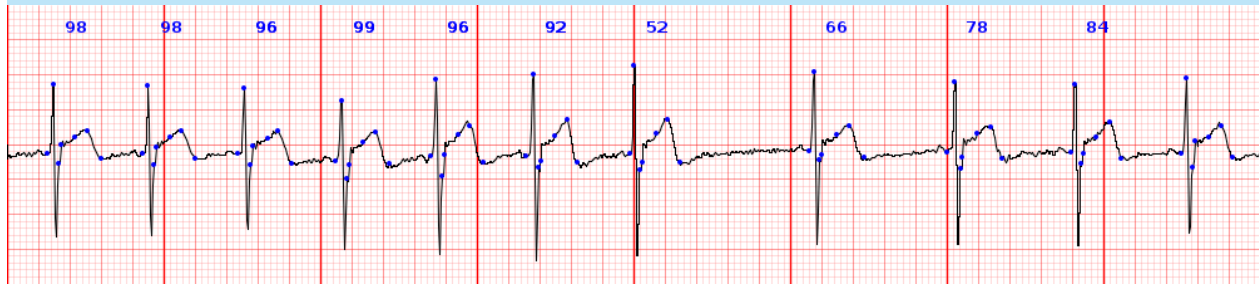


Minimum HR: 52 bpm
at 01-01-2026 14:58:48

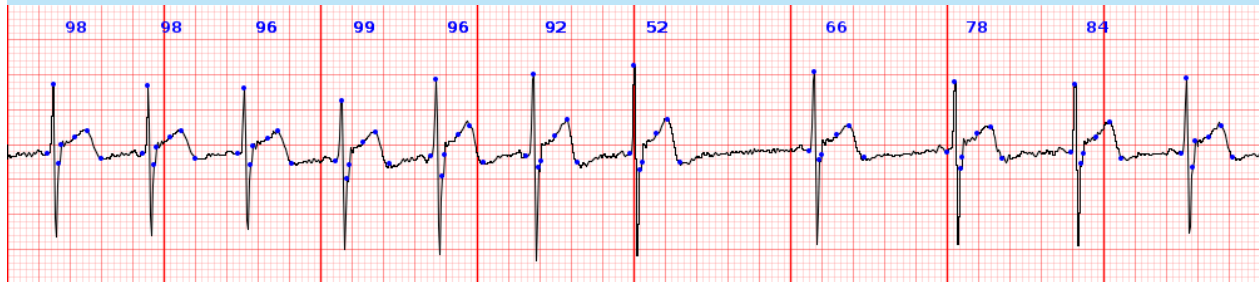


Maximum HR: 120 bpm
at 01-01-2026 15:01:06

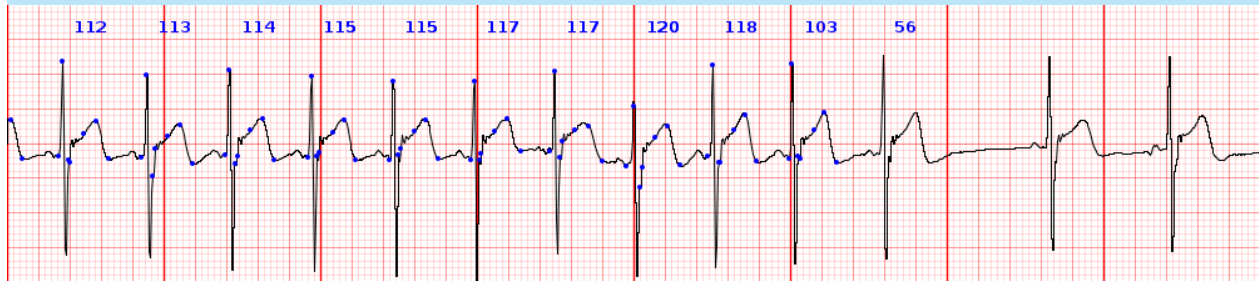

Lowest 1-minute meanHR: 72 bpm
(16:01:09 – 16:02:10)

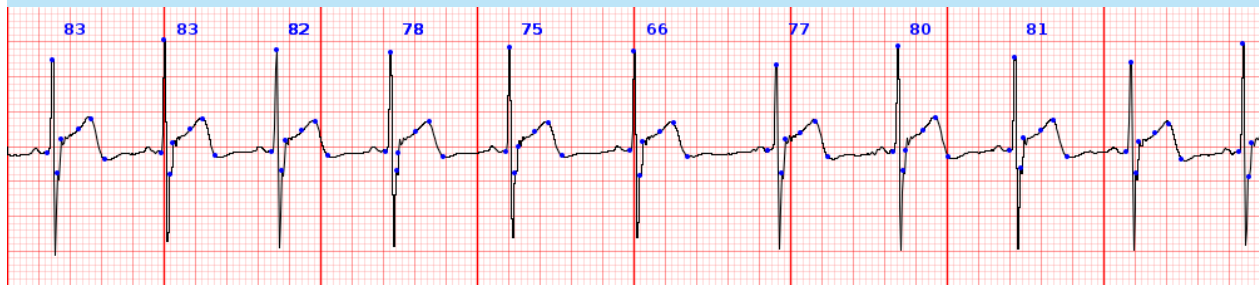

HR over time

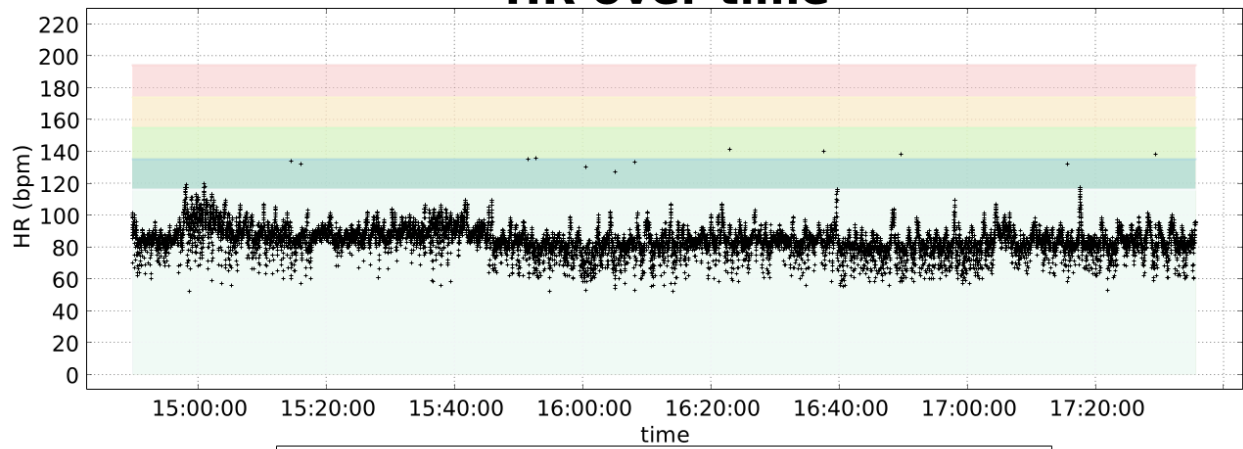


— Maximum, 90-100% HR max., 175-194 bpm, for: 0 minutes
— Anaerobic, 80-90% HR max., 156-174 bpm, for: 0 minutes
— Aerobic, 70-80% HR max., 136-155 bpm, for: 0 minutes
— Recovery, 60-70% HR max., 117-135 bpm, for: 0 minutes
Rest zone < 60% HR max., <116 bpm, for: 164 minutes
· HR, Heart Rate

Heart Rate Effort Index





26

Heart Rate Variability (HRV)


54

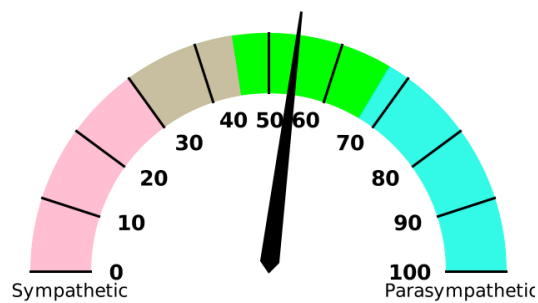


Reference interval according to age is
[45-67] approximately

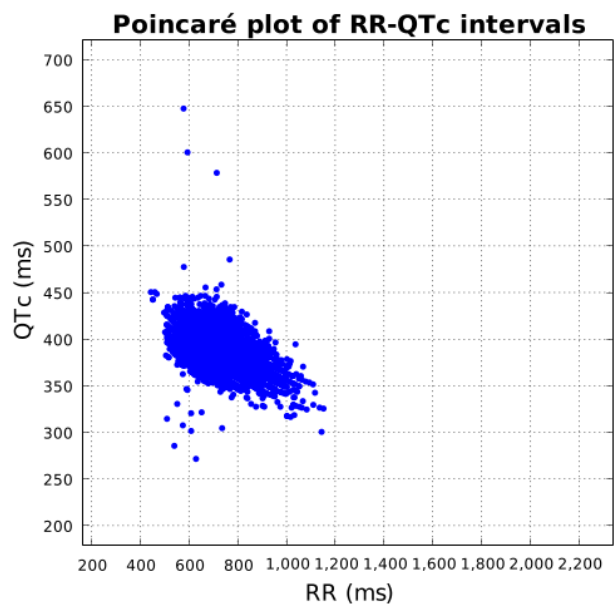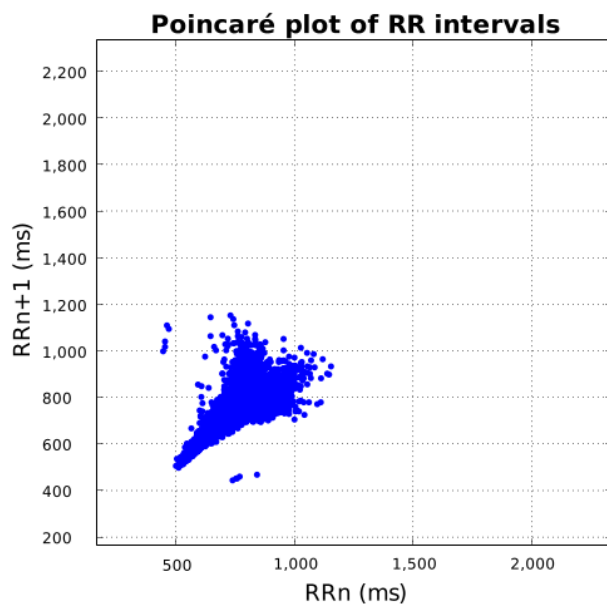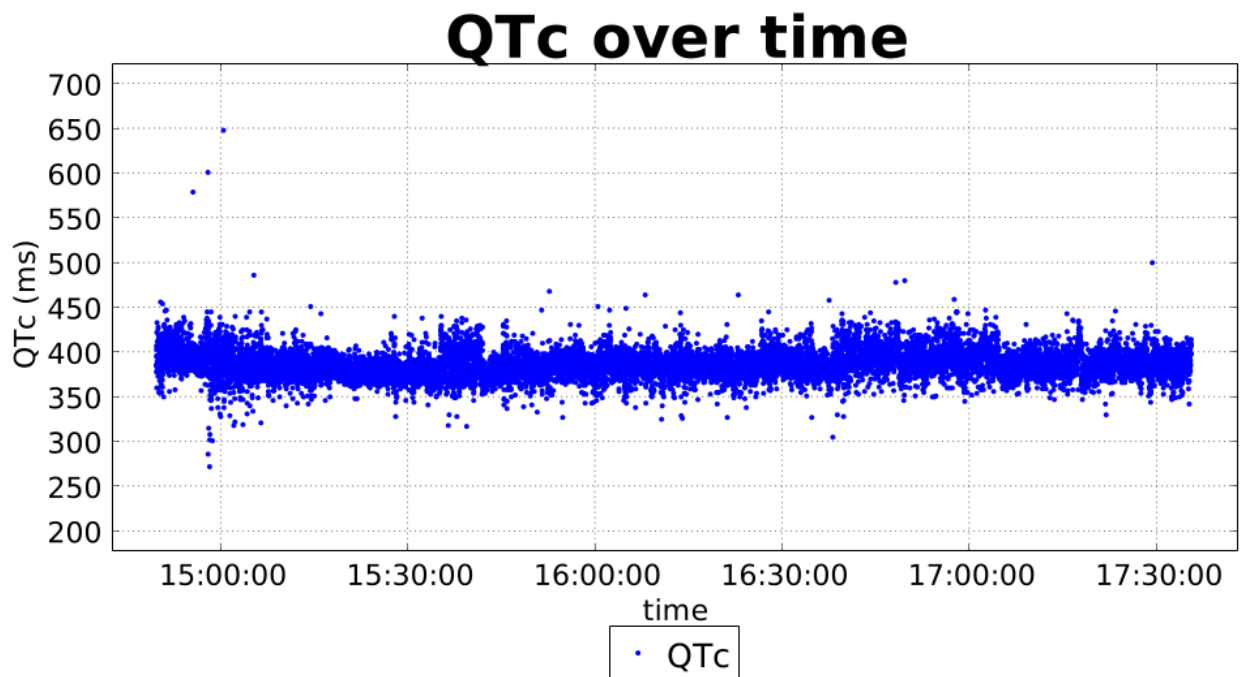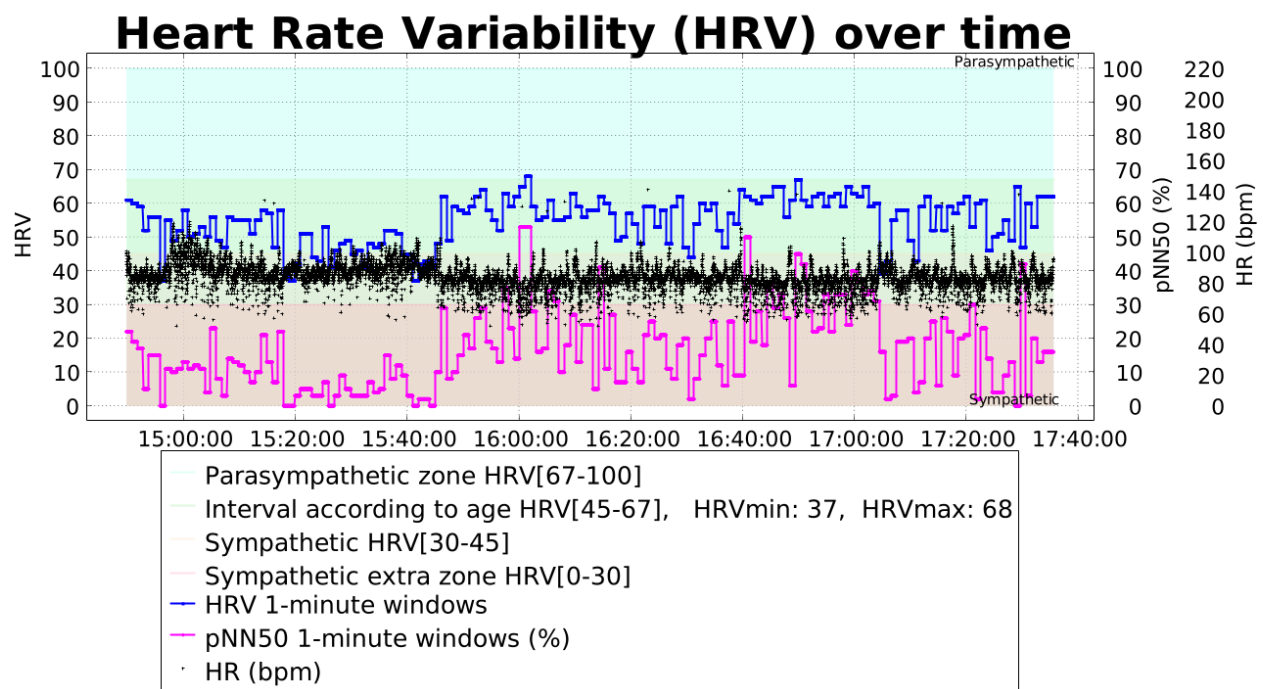


Event 01-01-2026 15:14:33 (1/10)

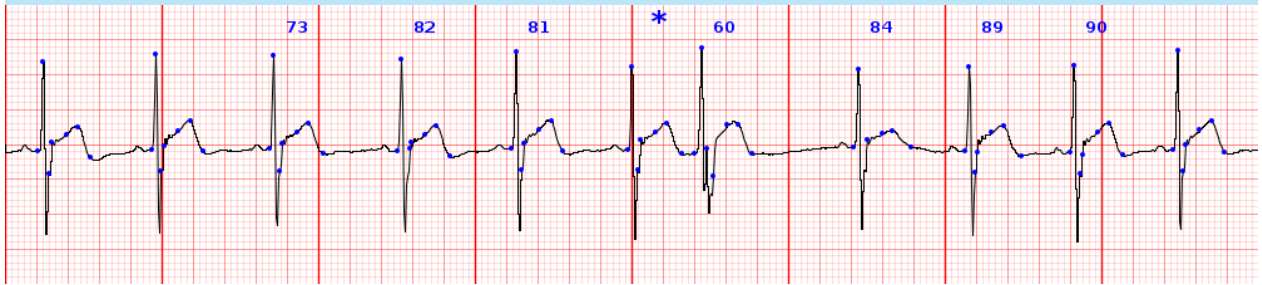


Event 01-01-2026 15:16:11 (2/10)

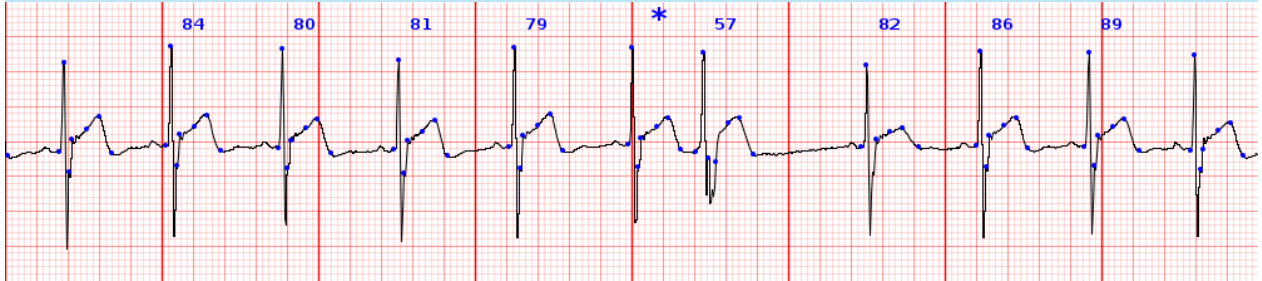


Event 01-01-2026 15:28:12 (3/10)

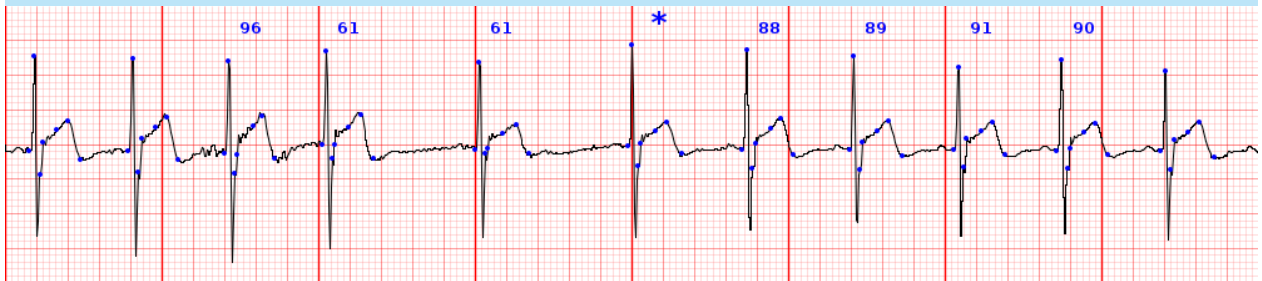


Event 01-01-2026 15:51:34 (4/10)

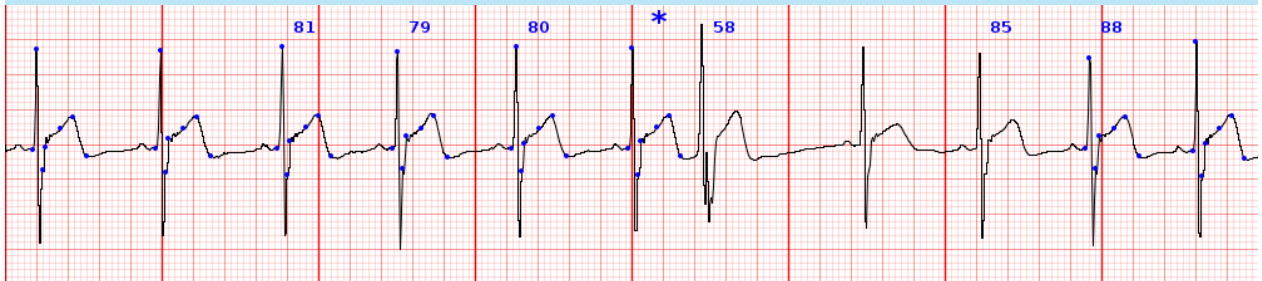


Event 01-01-2026 15:52:49 (5/10)

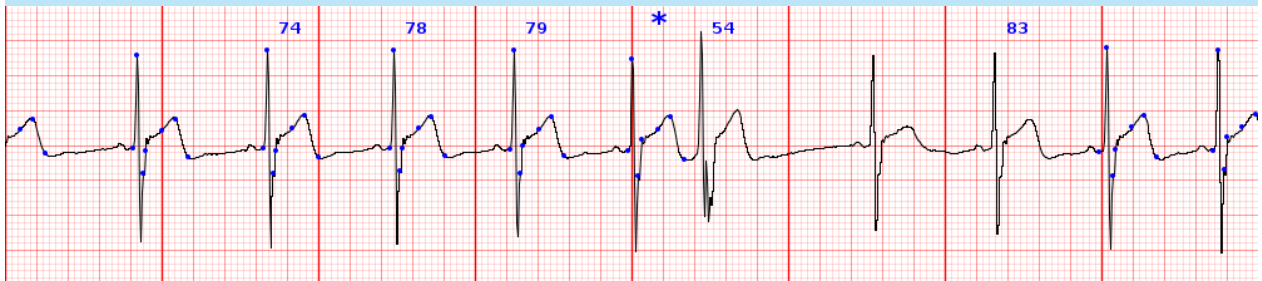


Event 01-01-2026 16:00:35 (6/10)

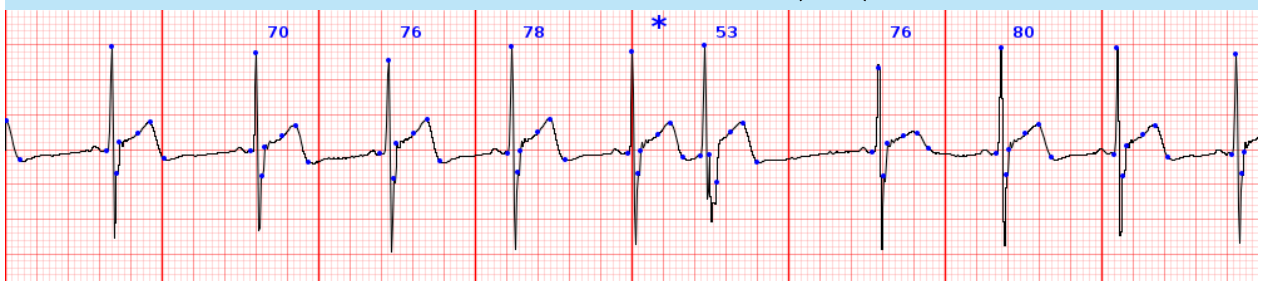


Event 01-01-2026 16:13:55 (7/10)

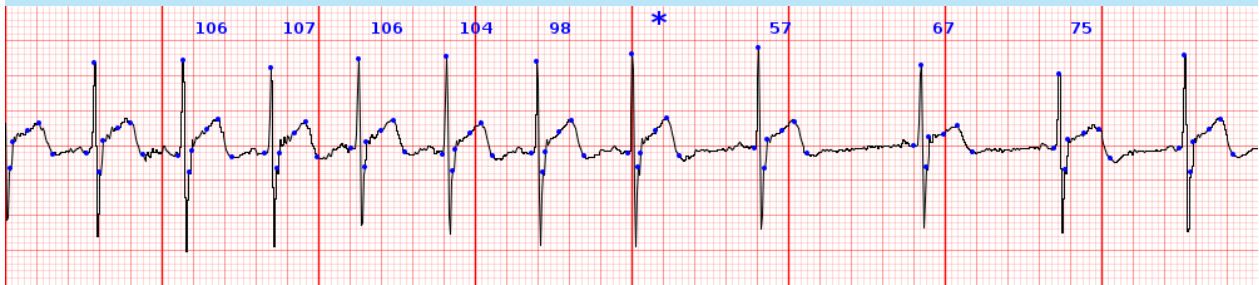


Event 01-01-2026 16:40:19 (8/10)

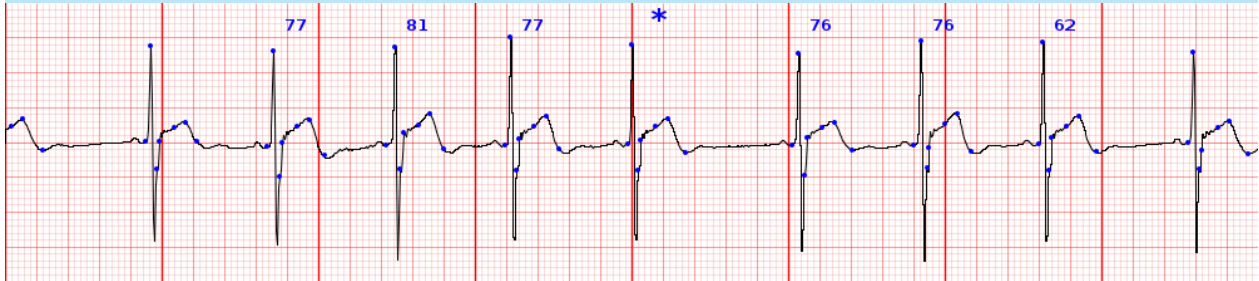

Event 01-01-2026 16:40:28 (9/10)

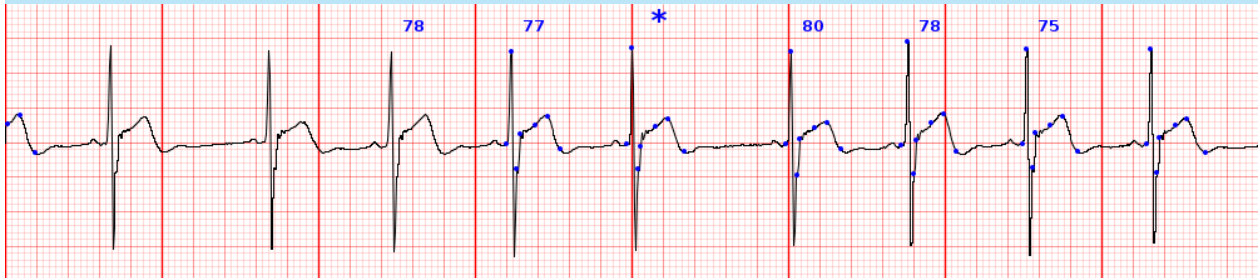

Event 01-01-2026 16:40:31 (10/10)

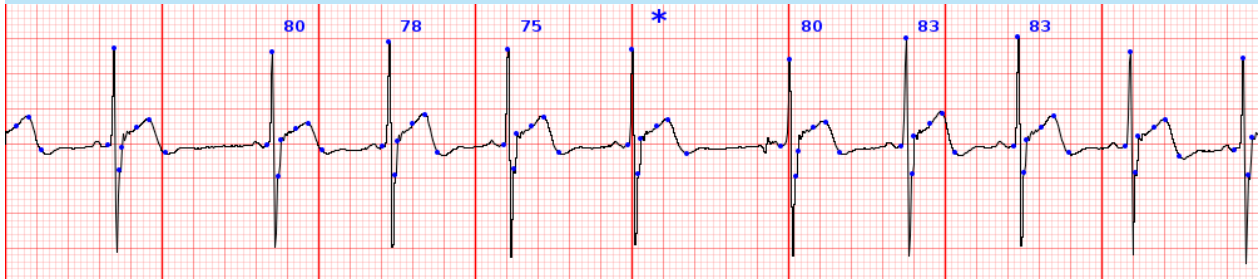

Upgrade subscription to see more Events

Event 01-01-2026 16:05:05

Event 01-01-2026 16:08:10

Event 01-01-2026 16:23:05

Event 01-01-2026 16:37:38

Event 01-01-2026 16:49:45

Event 01-01-2026 17:15:45

Event 01-01-2026 17:29:26

Sensor information

Battery level	100%
Firmware version	3.3.1

new feature



(<https://biosignalssolutions.com/beatexplorerhelp>)

The new web application **BeatExplorer** provides users with the ability to access cloud-stored reports generated by the *Polar ECG Analysis* App. This web platform facilitates users and their specialists to examine remotely metrics and visualize trend graphs.

Click to know more
(<https://biosignalssolutions.com/beatexplorerhelp>)

Important notice: The use of the app and site is not intended to be a substitute for professional medical advice, diagnosis, treatment, or prevention of any disease or health condition. If you are concerned about your health, consult a medical specialist immediately. THE APP AND WEB SITE DO NOT OFFER MEDICAL ADVICE. The results are statistical, based on automated analysis and could be incorrect.

Made with ❤️ to empower you, from biosignalssolutions.com (<http://biosignalssolutions.com>)

v3.28.2 ej

Copyright (c) 2025 Biosignals Solutions