




TCN19-120, normalized during counting

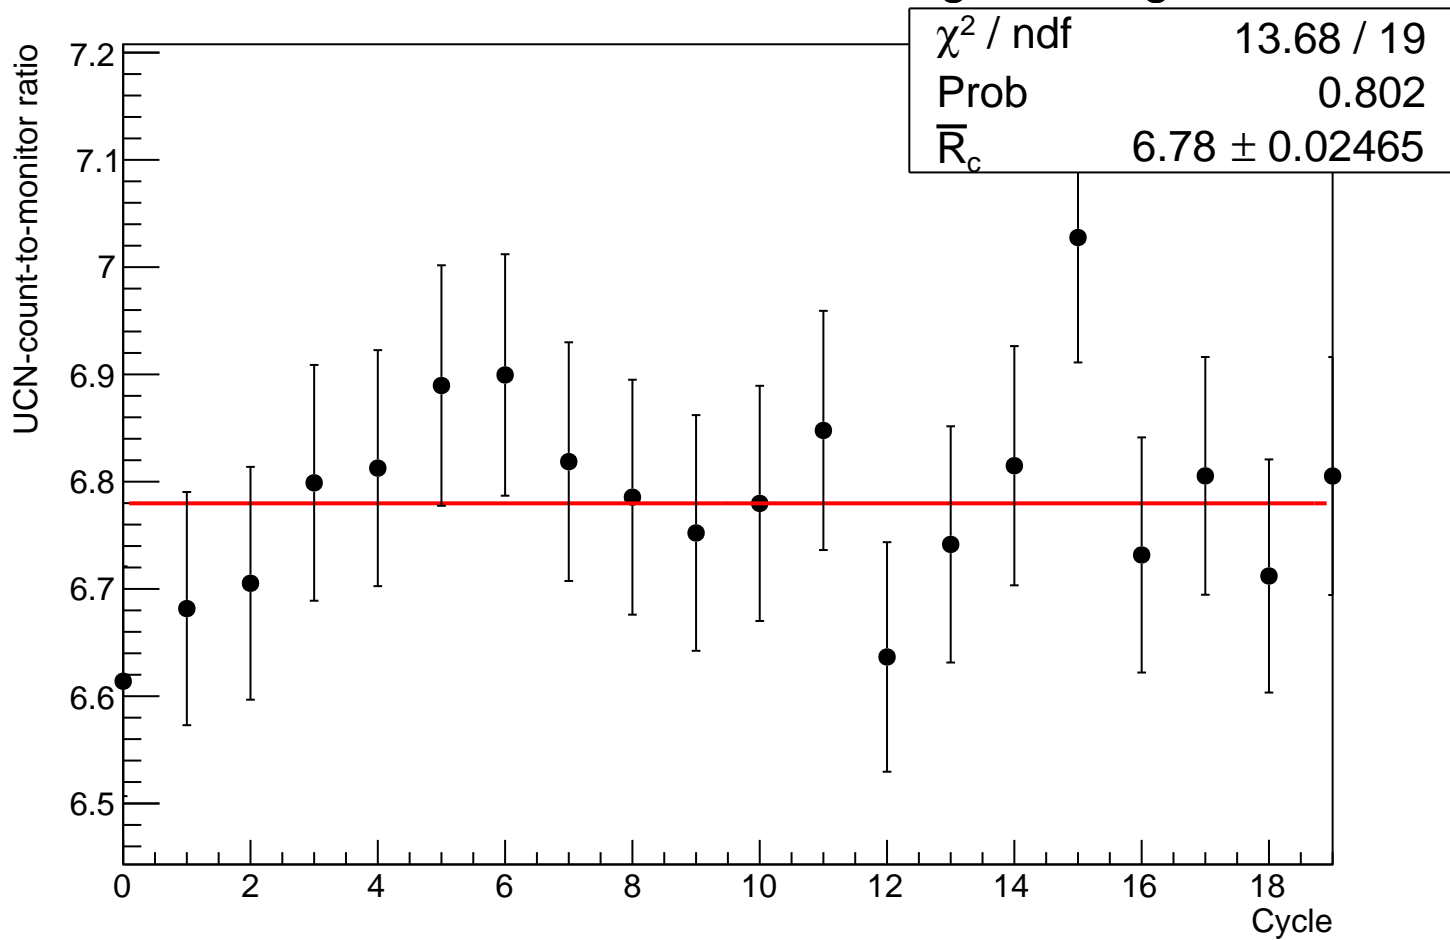



TCN19-120, normalized during irradiation

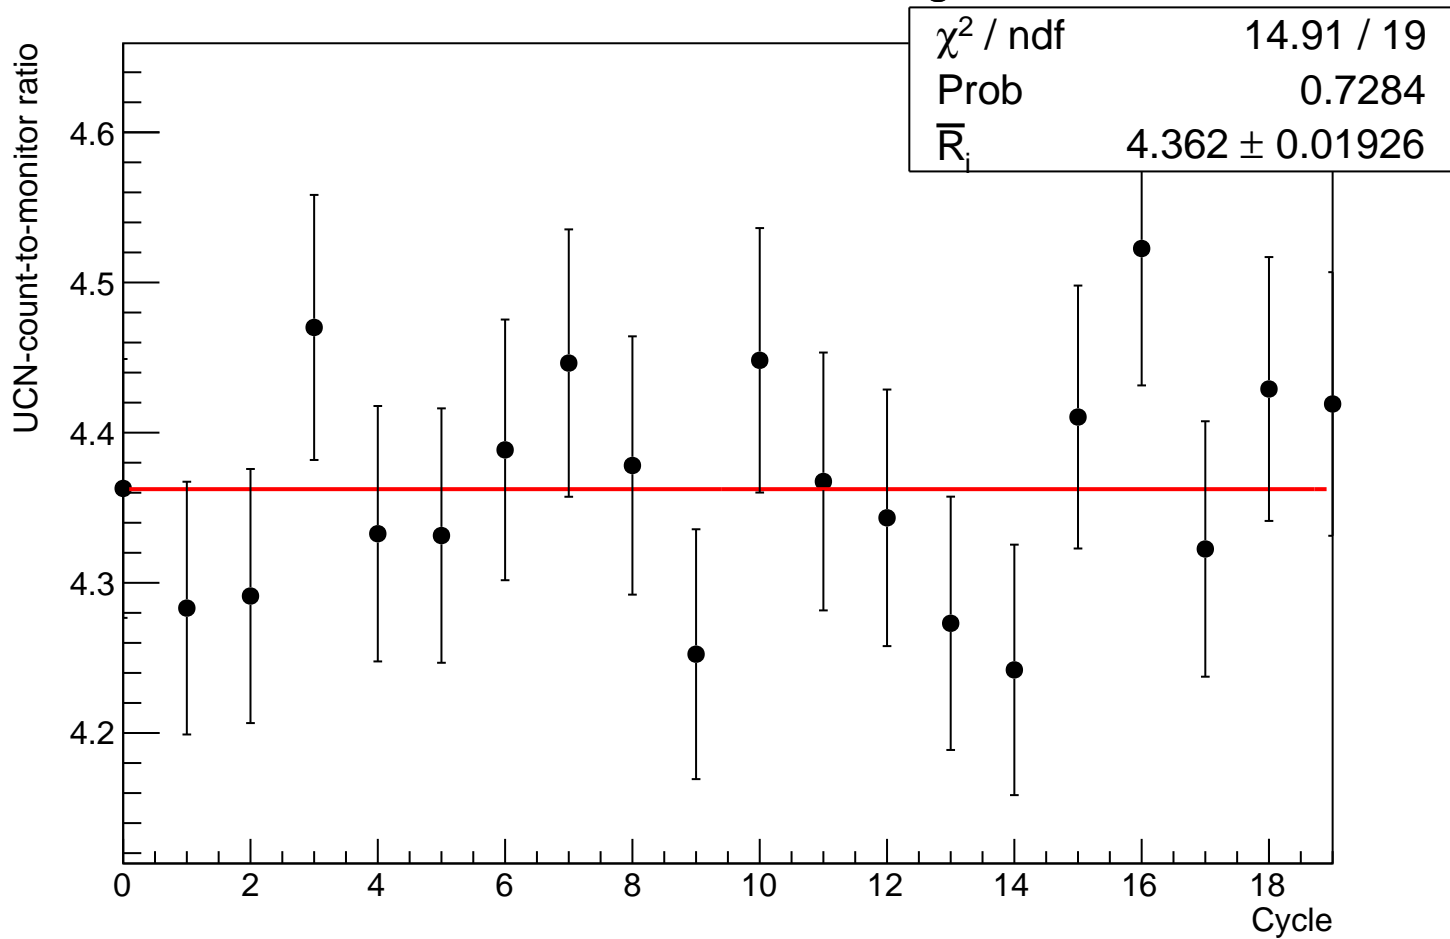


Graph

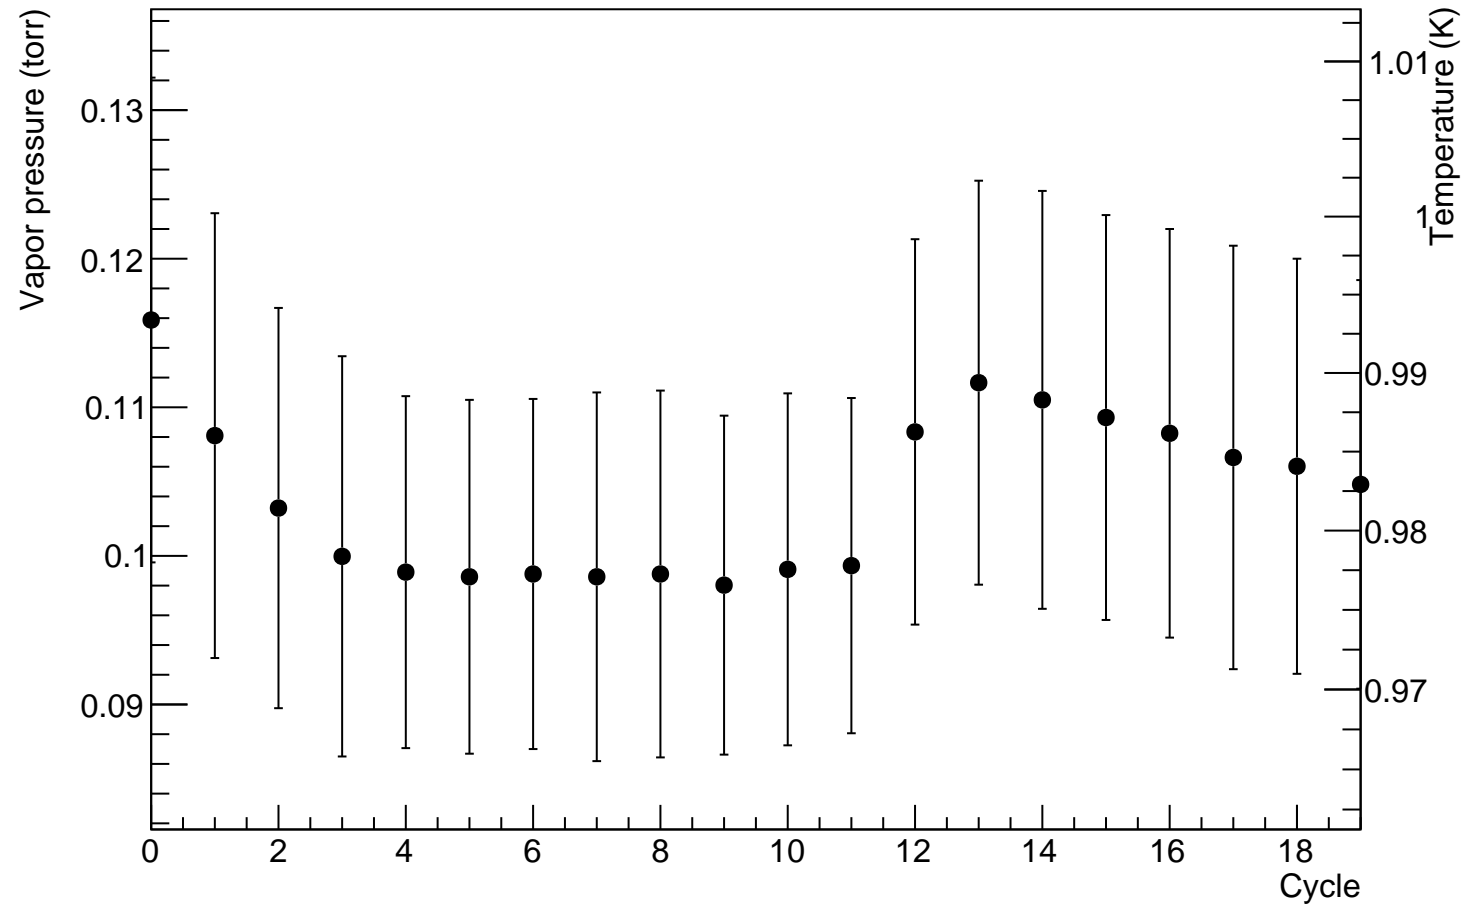


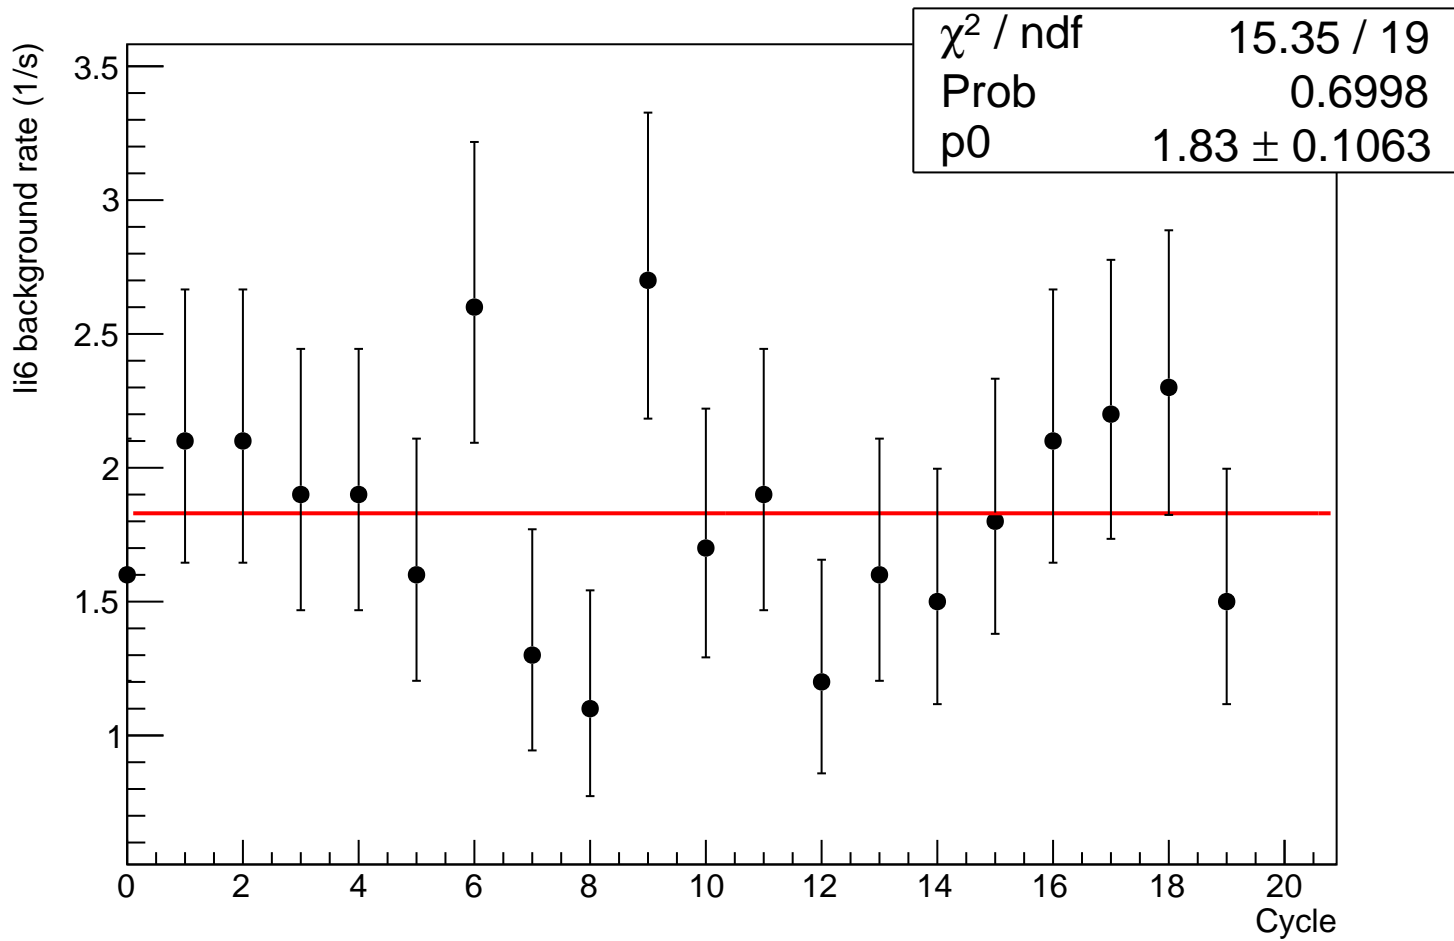

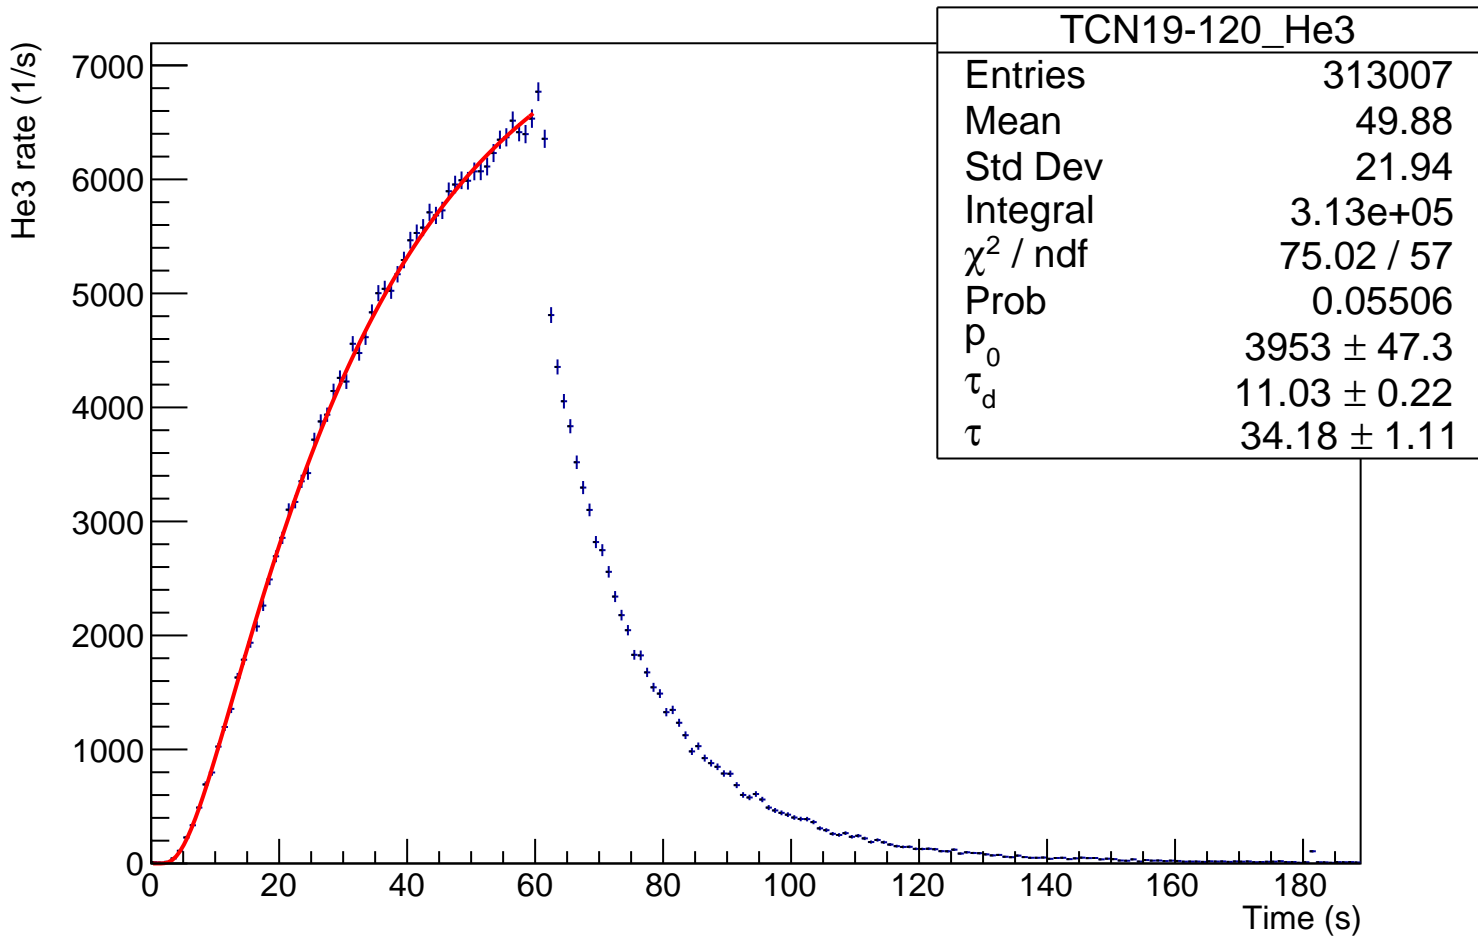

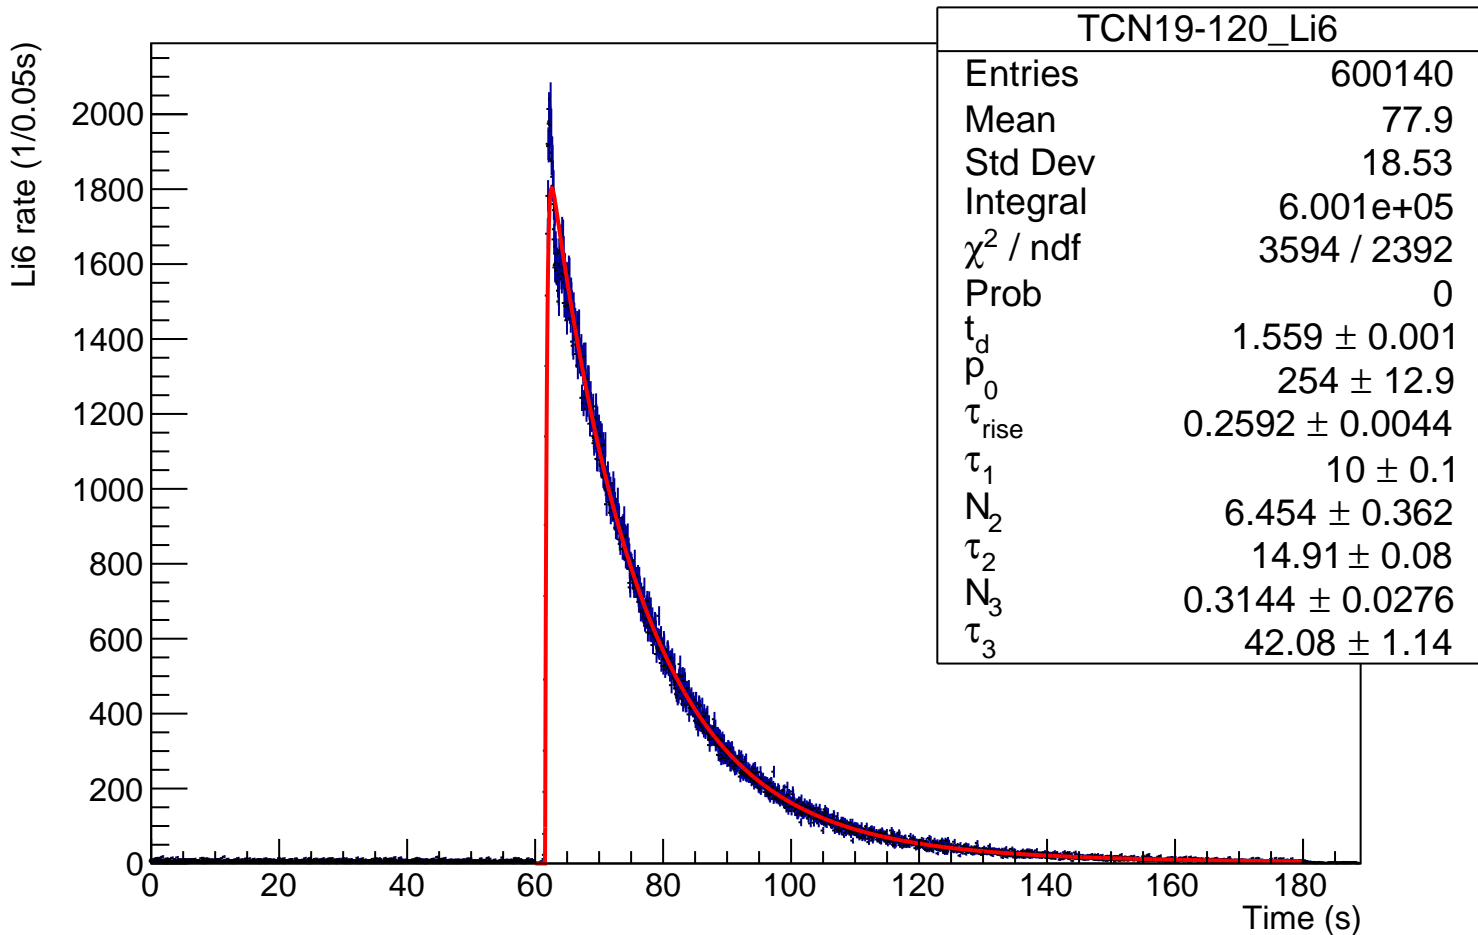

Li6 rate normalized during counting (1/0.05s)

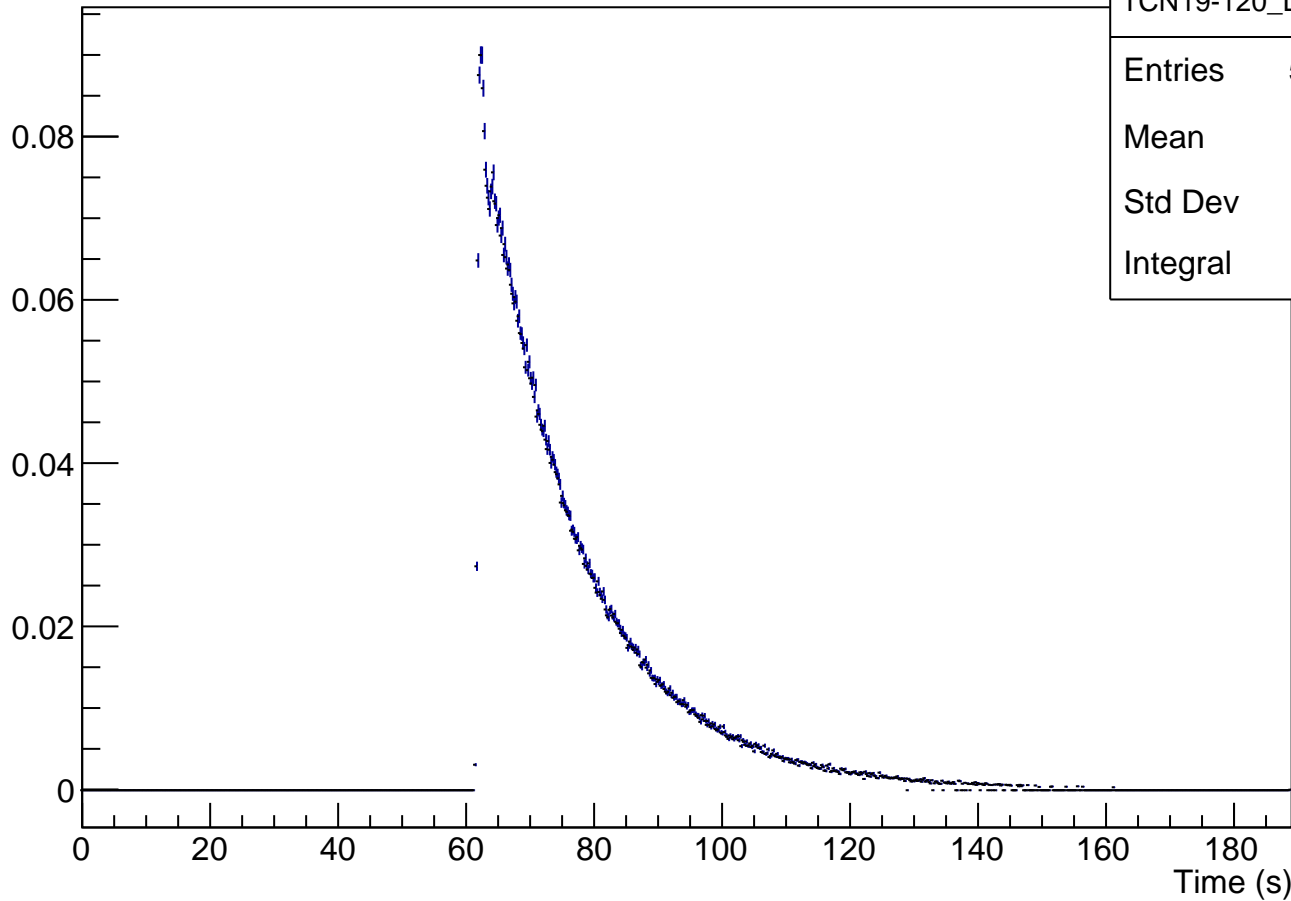

TCN19-120_Li6_norm


Entries 565108


Mean 77.74


Std Dev 17.76

Integral 6.576

Li6 rate normalized during irradiation (1/0.05s)

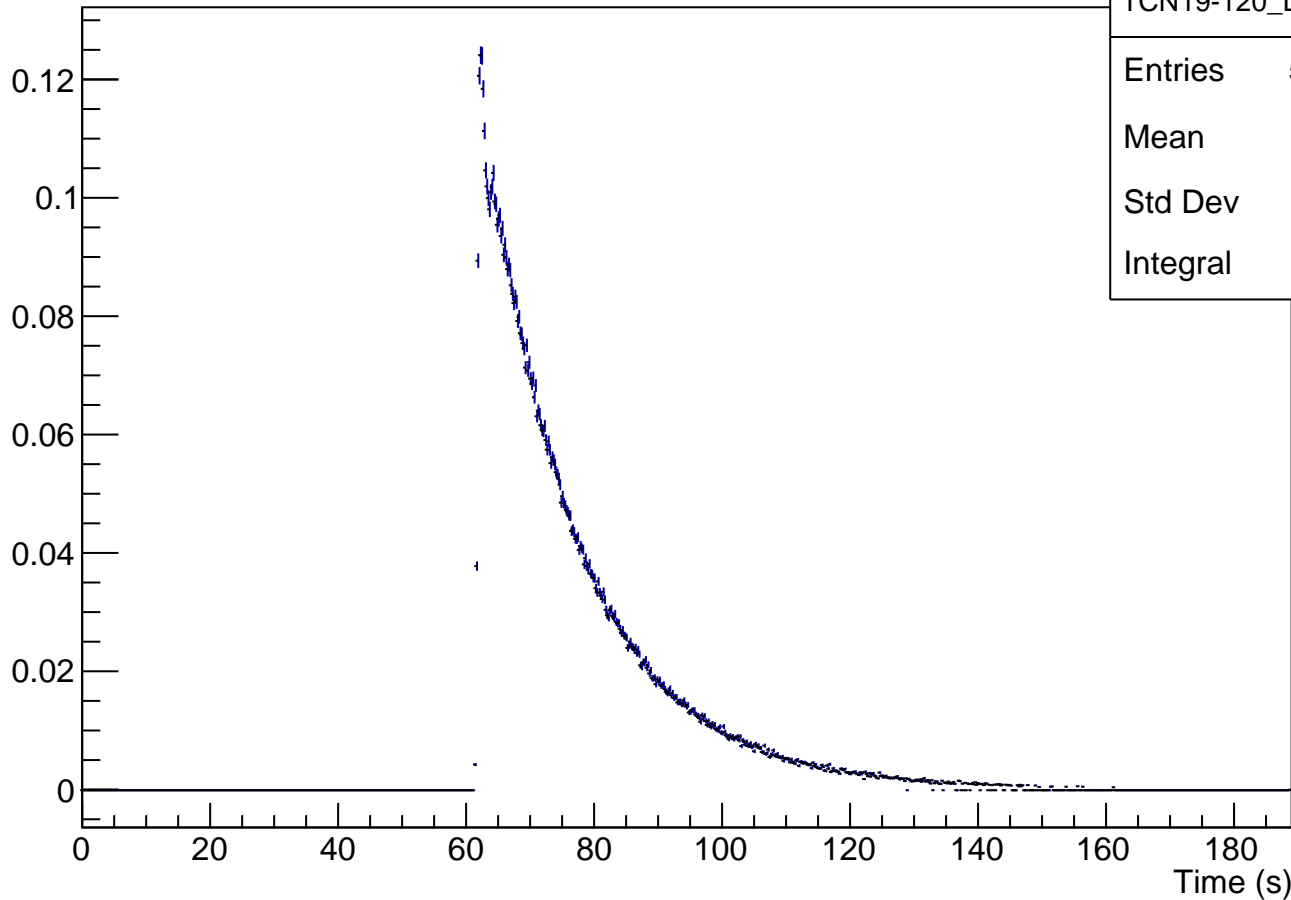


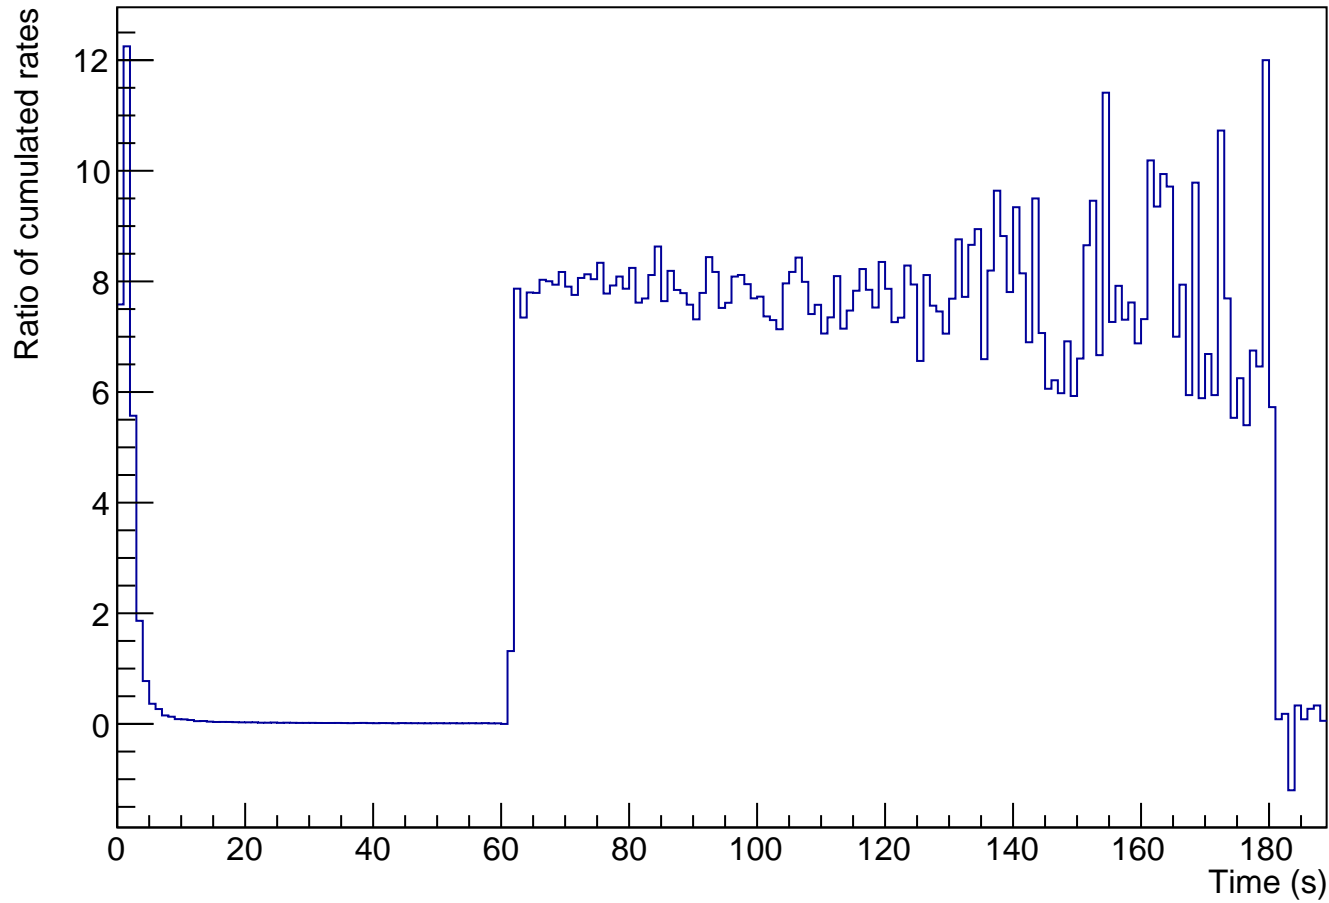

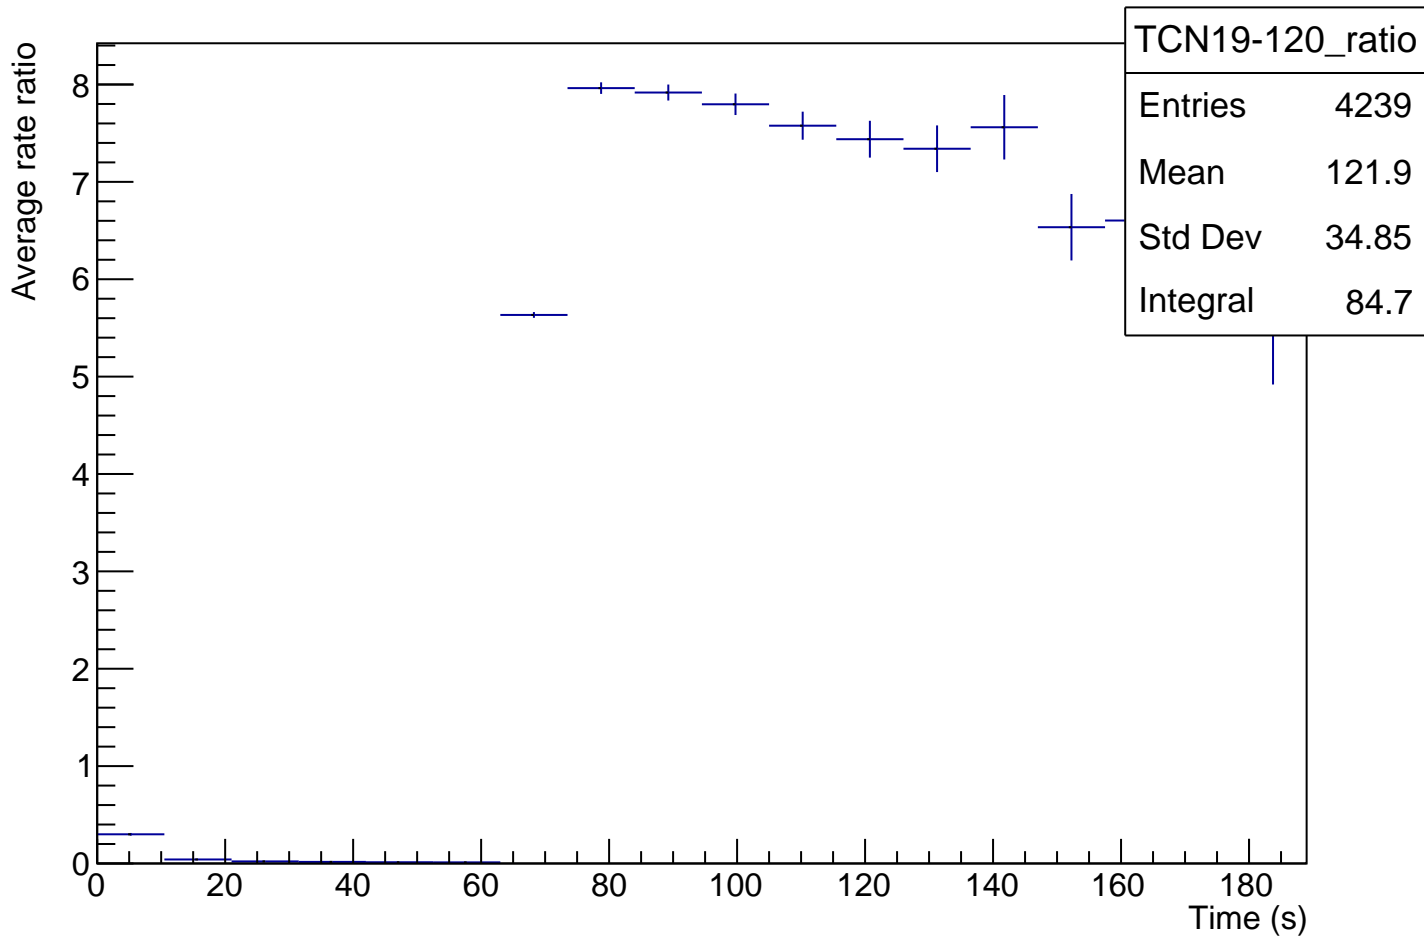

TCN19-120

Count

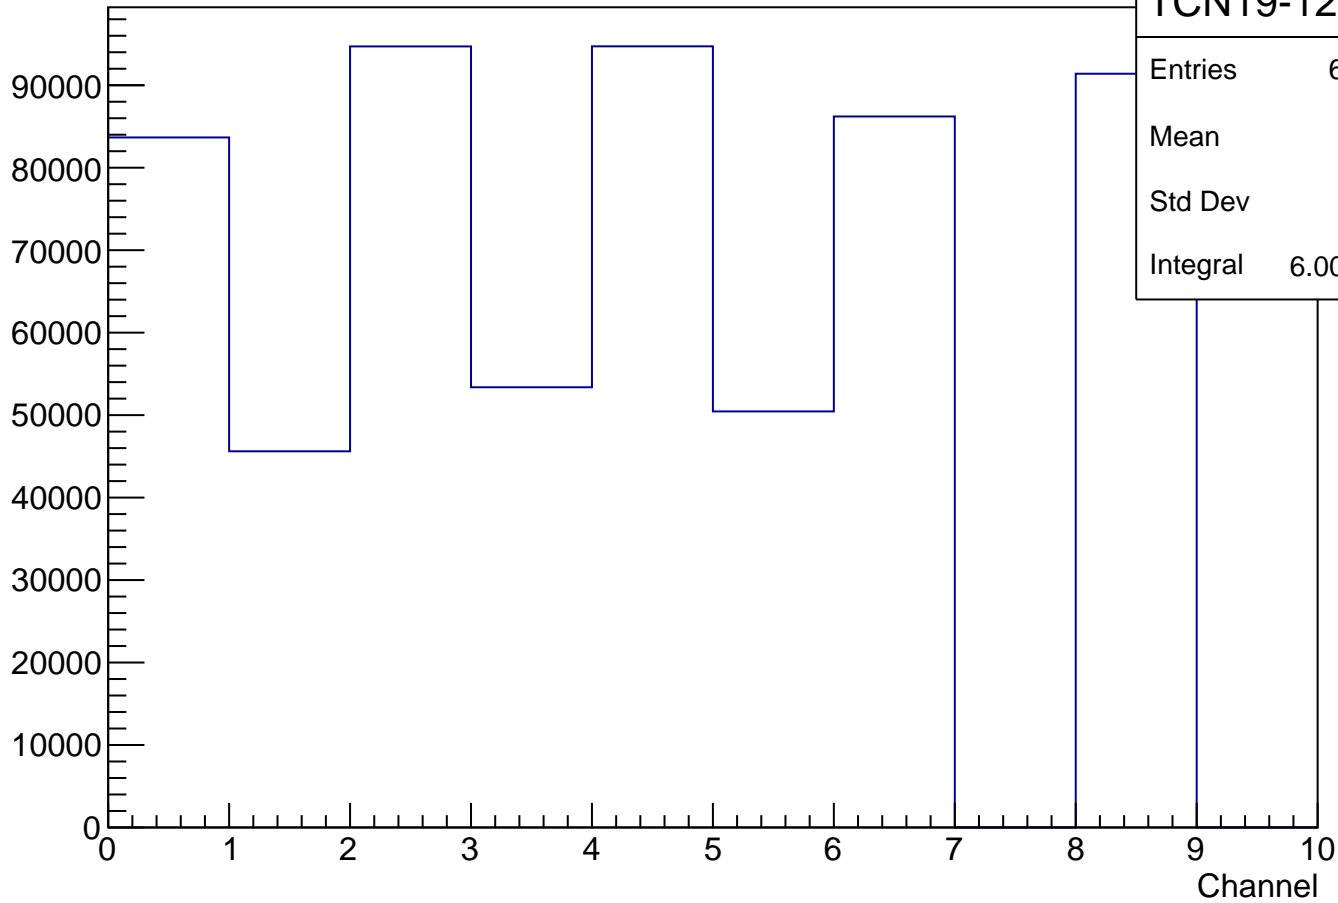

TCN19-120_ch

Entries 600140


Mean 3.79

Std Dev 2.586

Integral 6.001e+05

Li6 window

Frequency

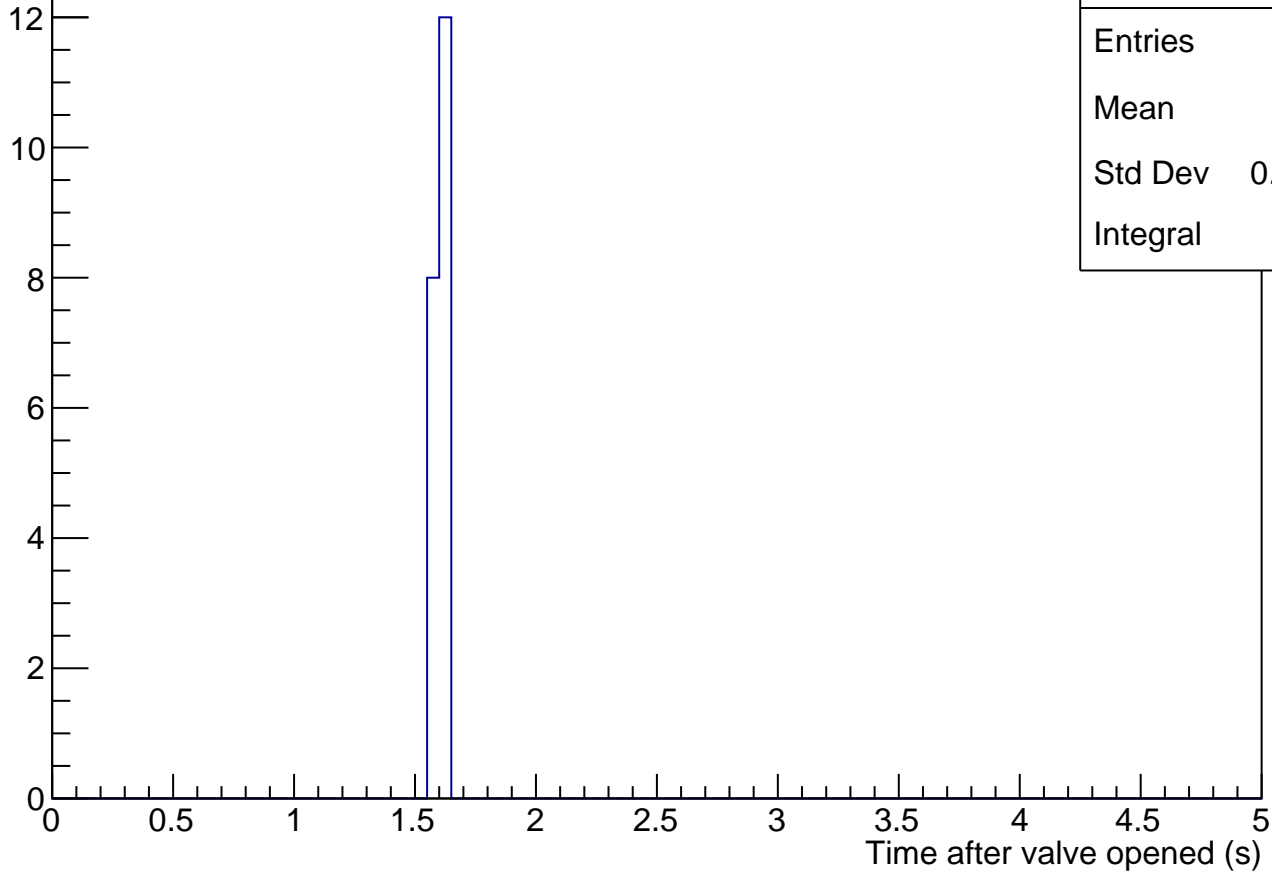

li6window

Entries	20
Mean	1.58
Std Dev	0.02449
Integral	20