




TCN19-120A, normalized during counting

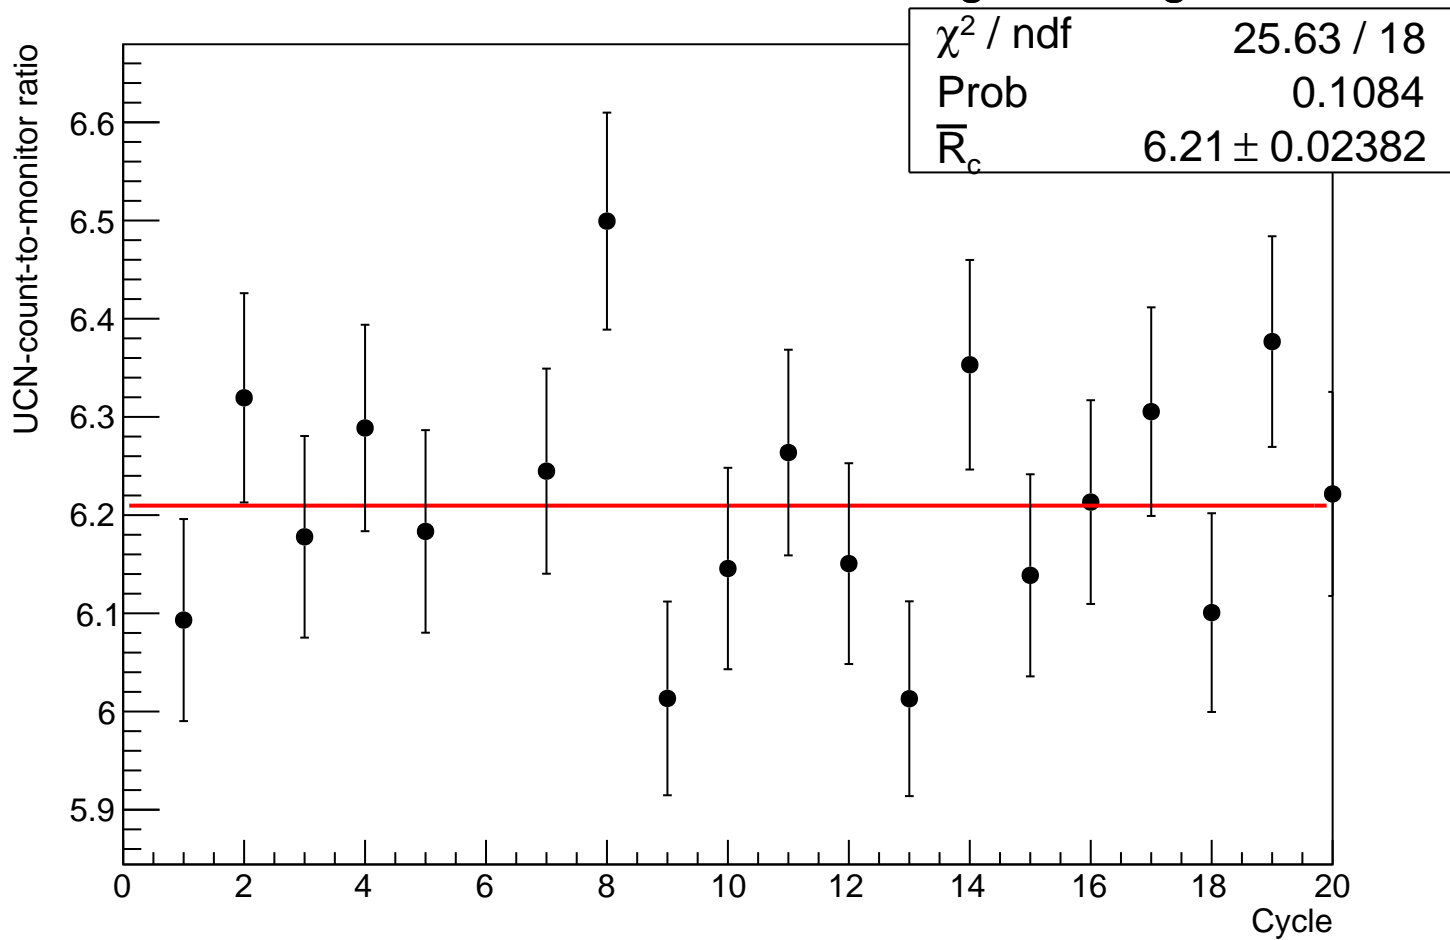



TCN19-120A, normalized during irradiation

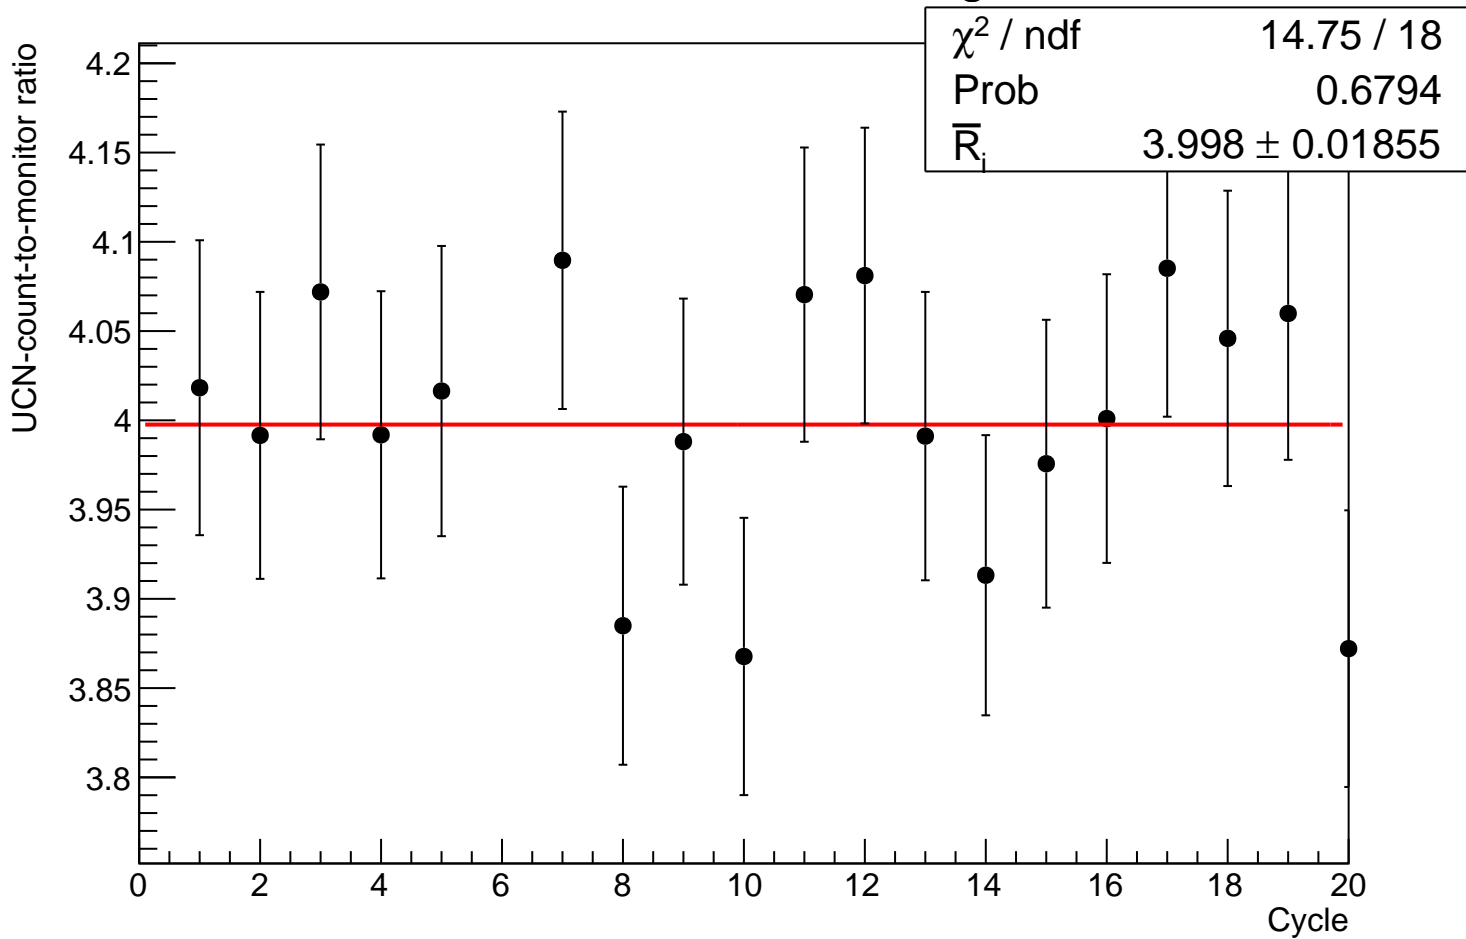


Graph

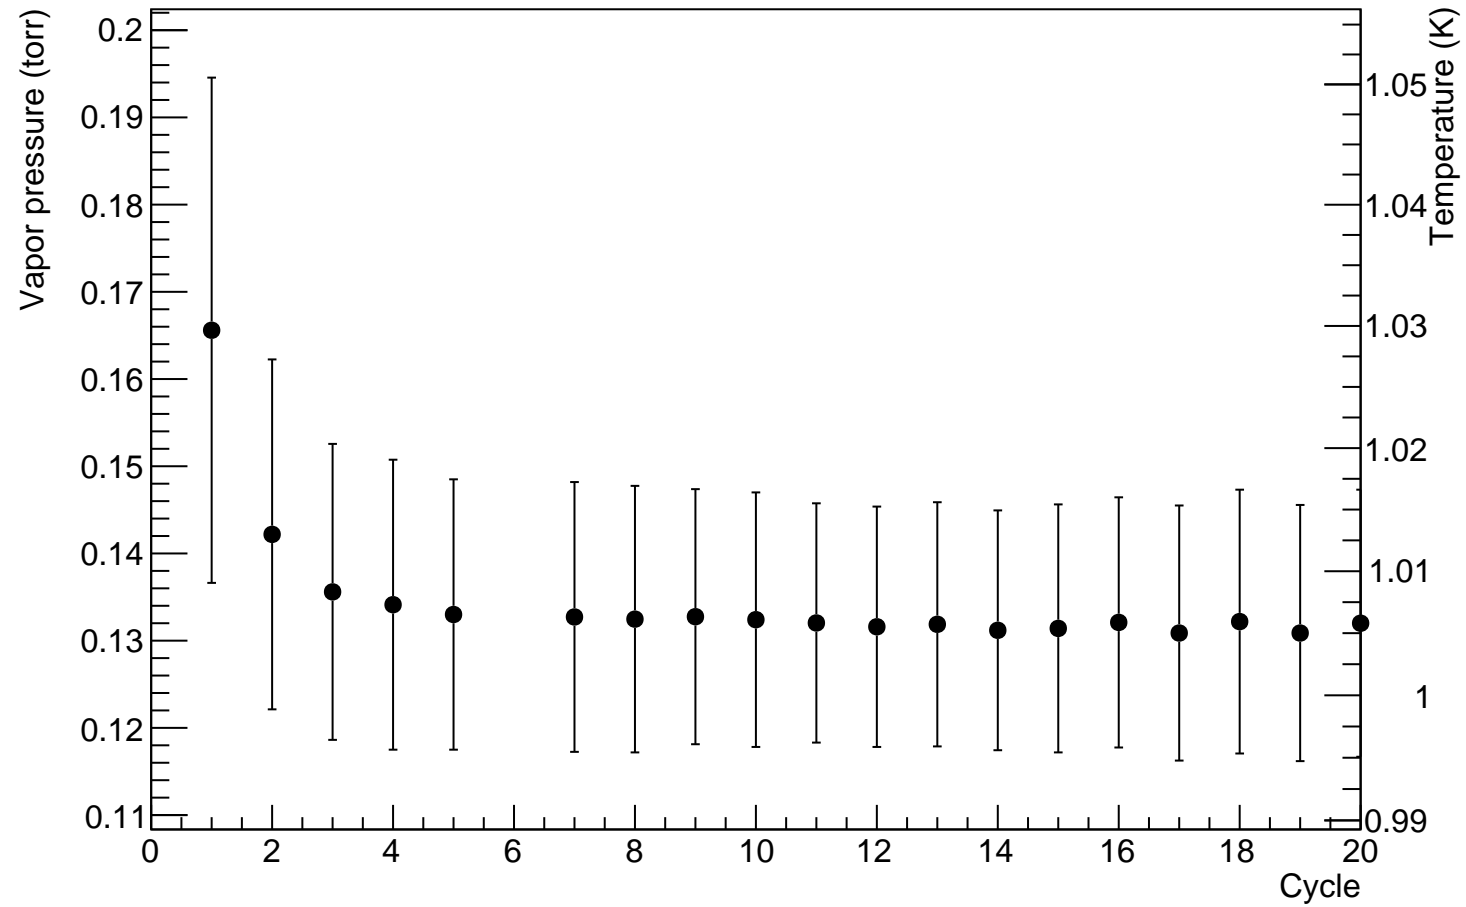


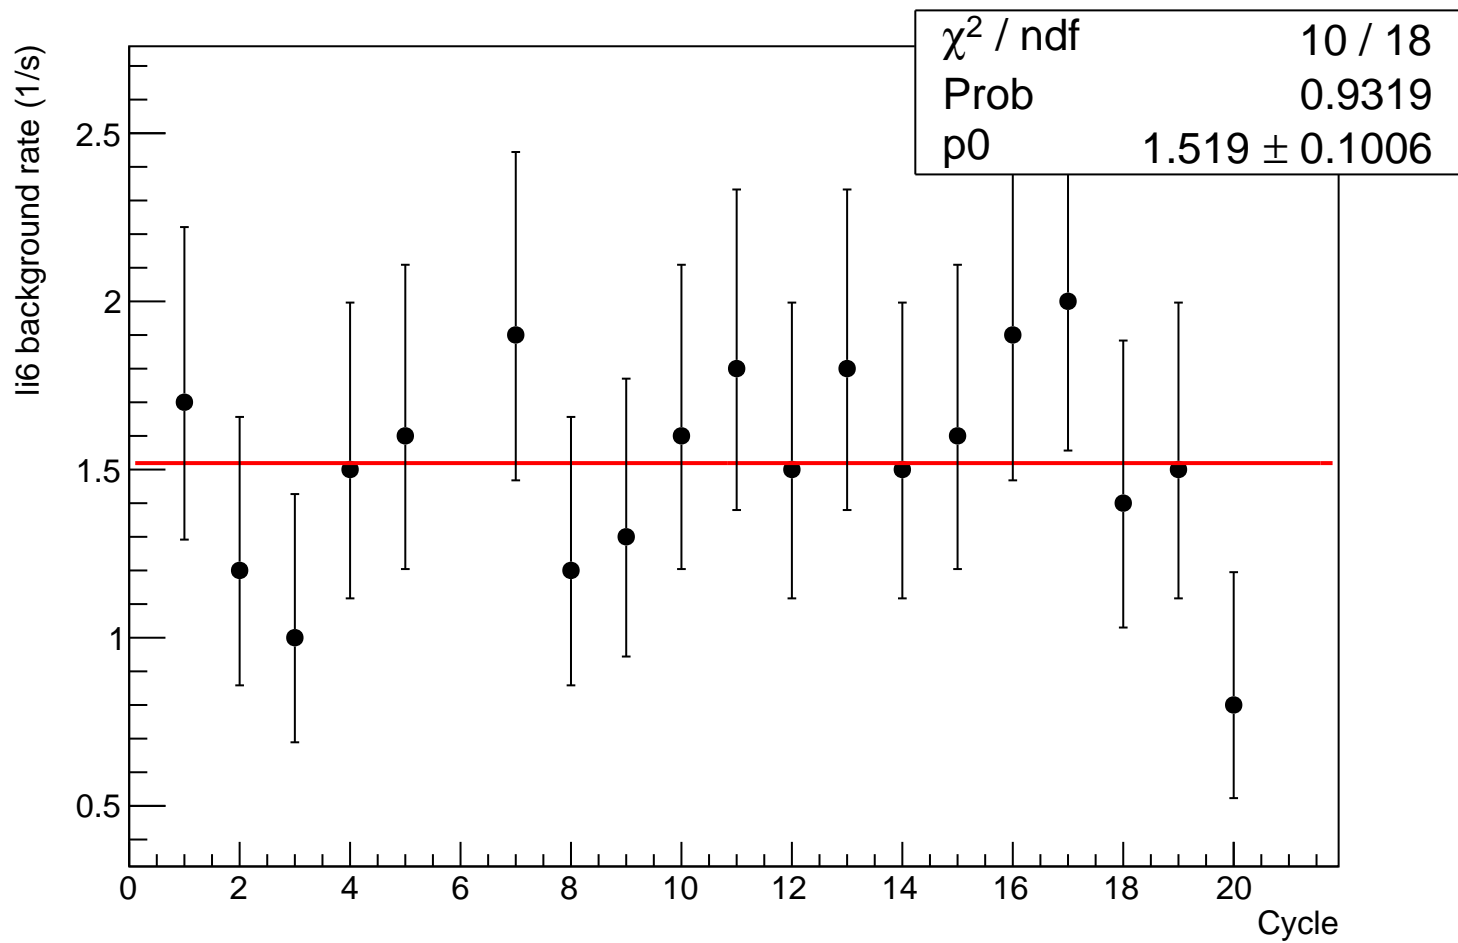

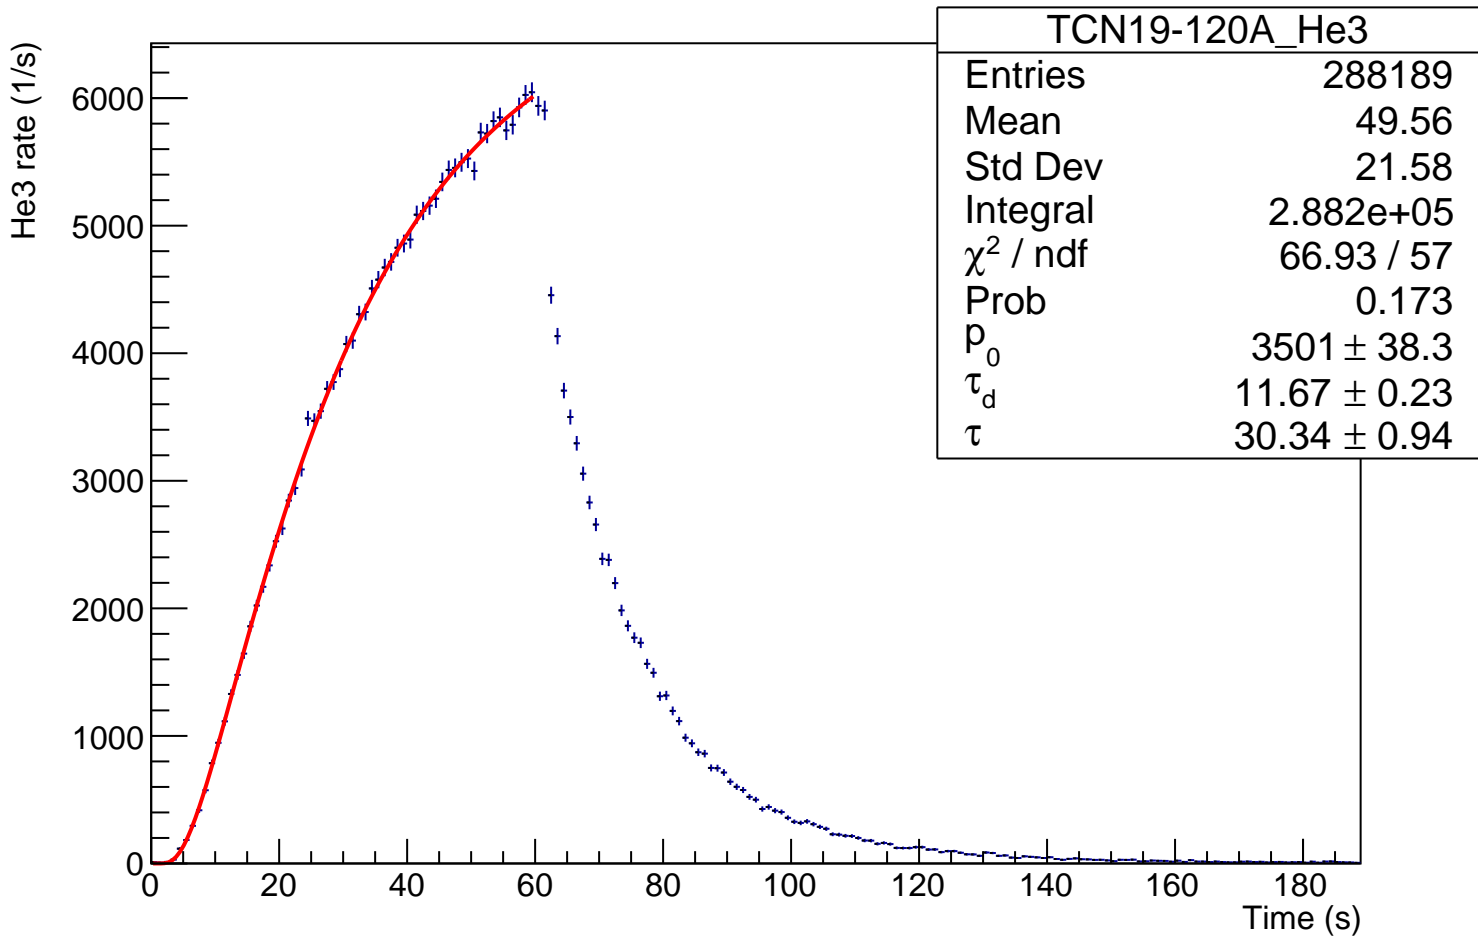

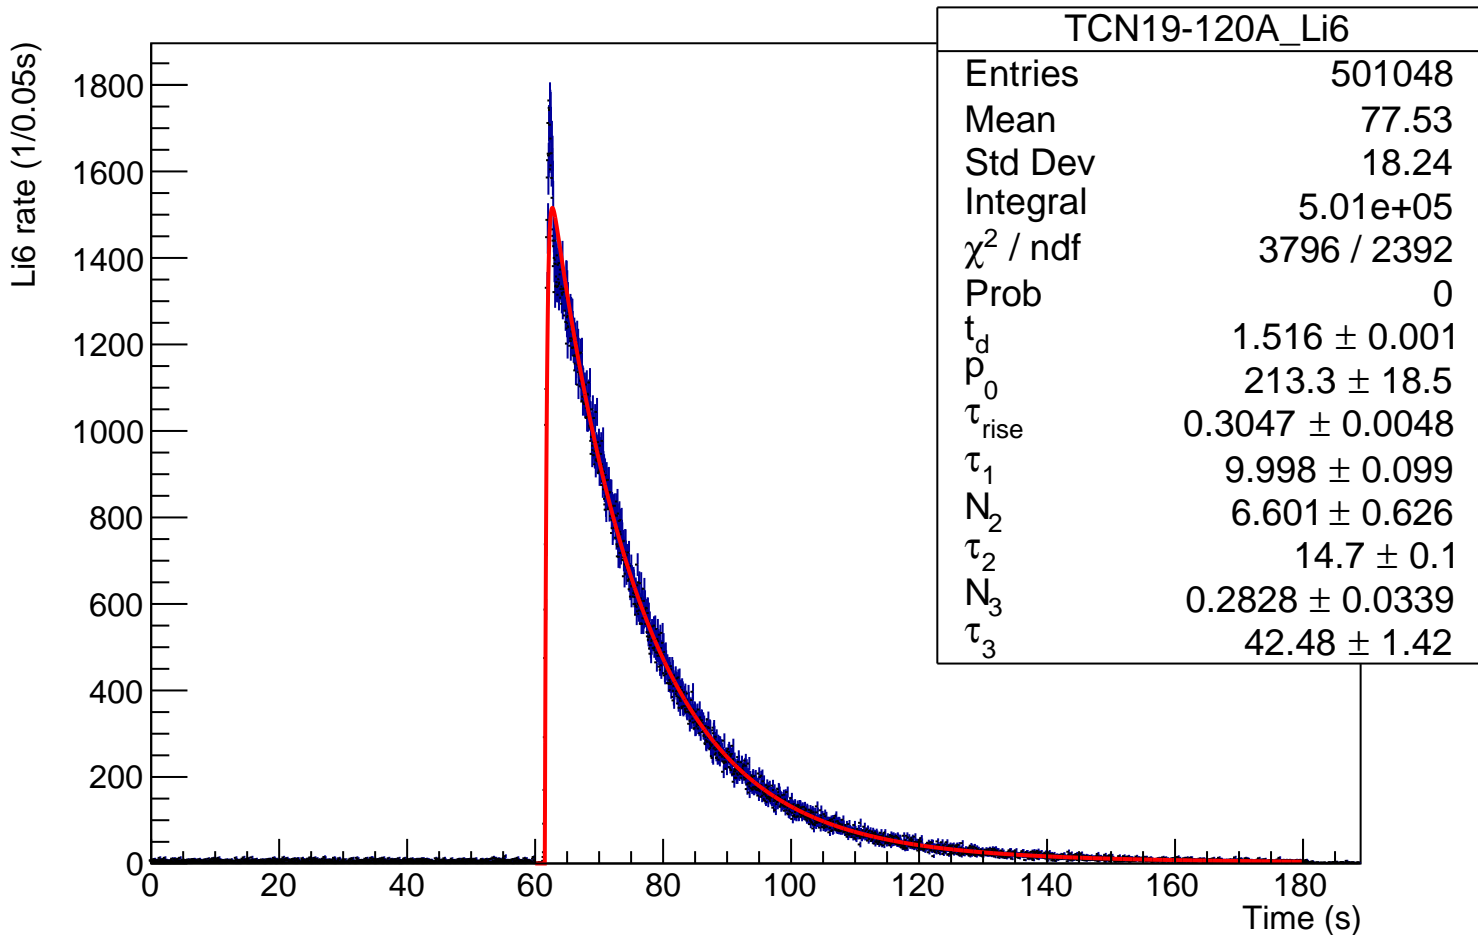

Li6 rate normalized during counting (1/0.05s)

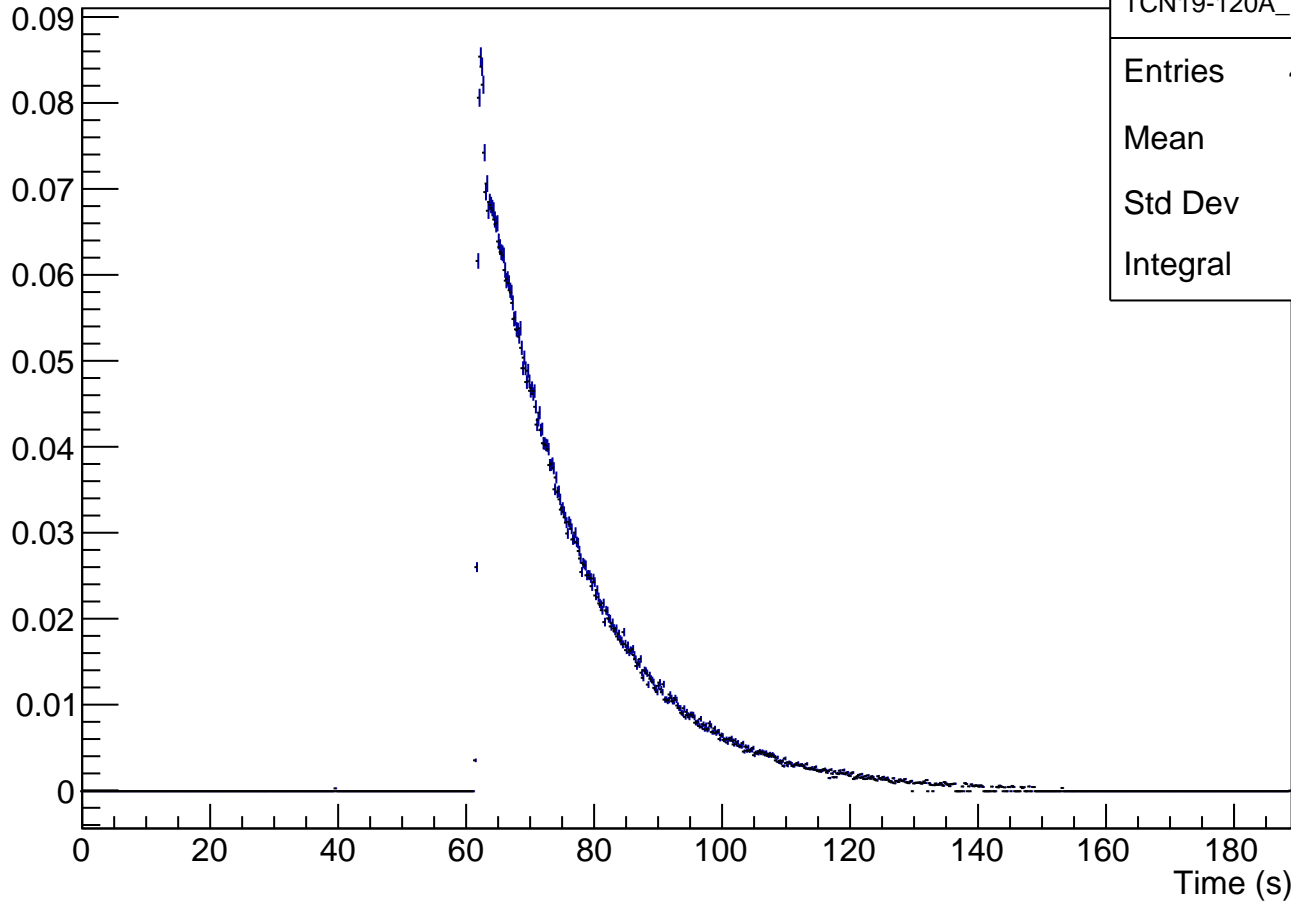

TCN19-120A_Li6_norm


Entries 471812

Mean 77.35


Std Dev 17.34


Integral 6.009

Li6 rate normalized during irradiation (1/0.05s)

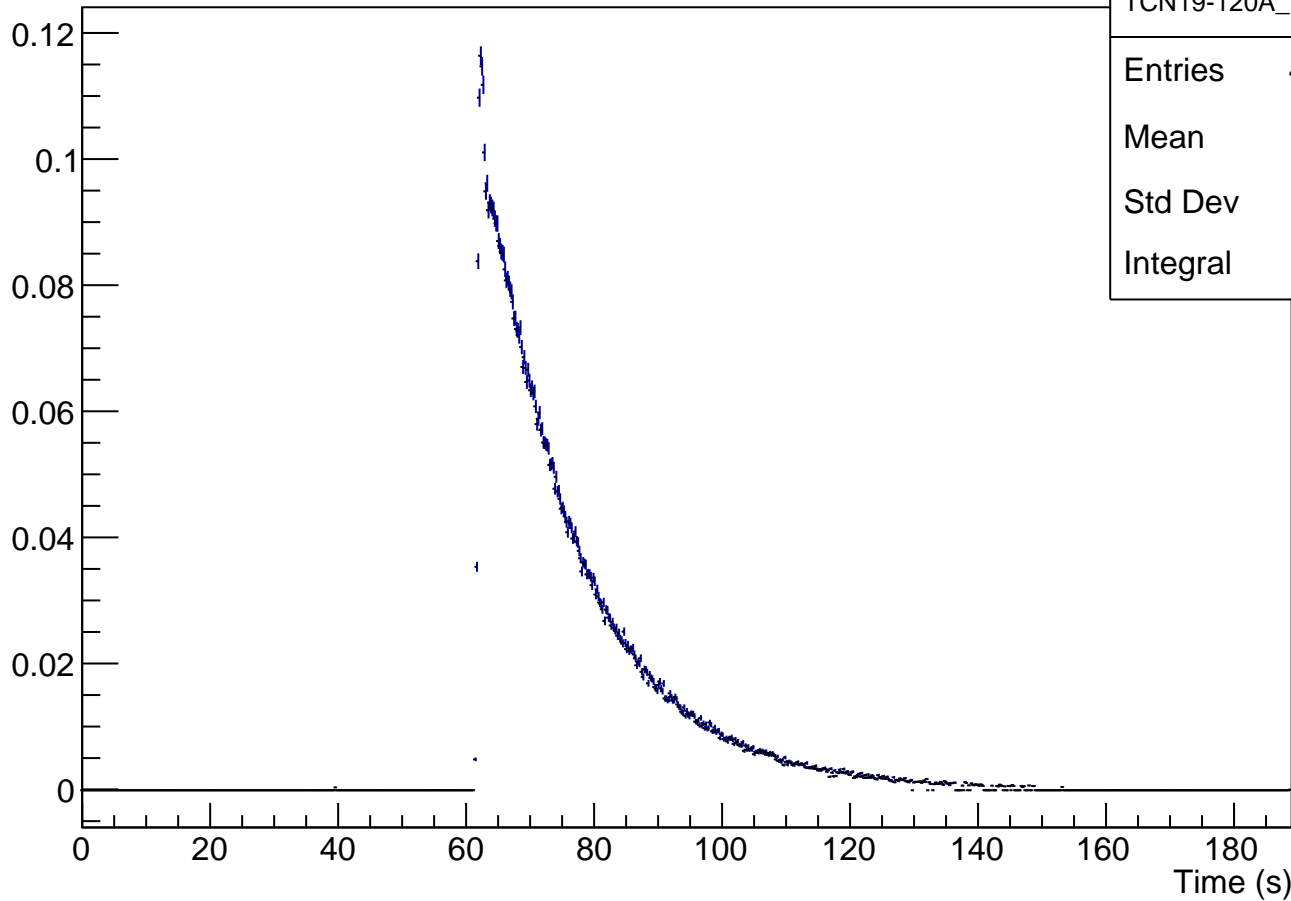


TCN19-120A_Li6_norm	
Entries	465466
Mean	77.35
Std Dev	17.34
Integral	8.183

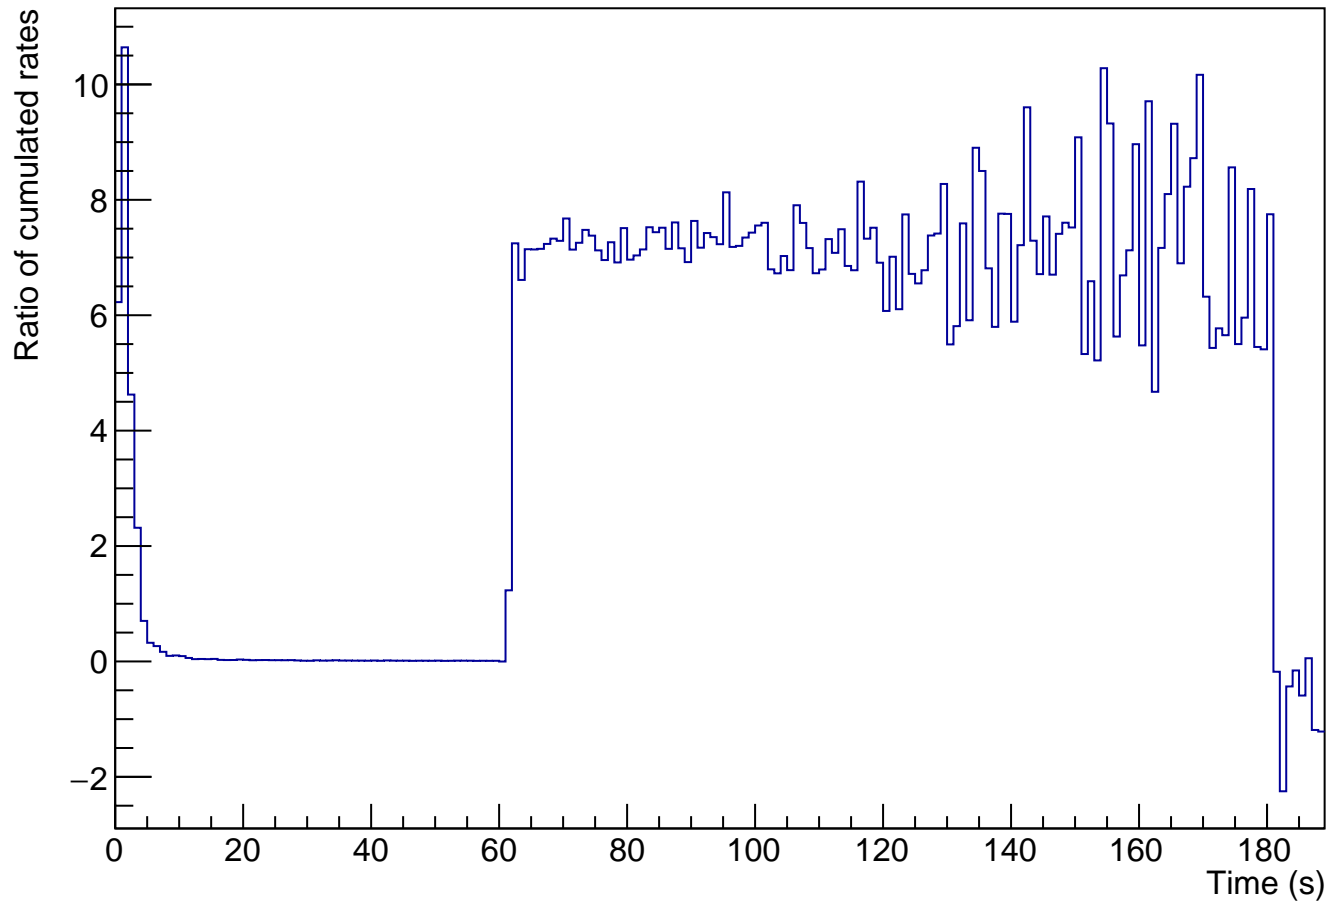

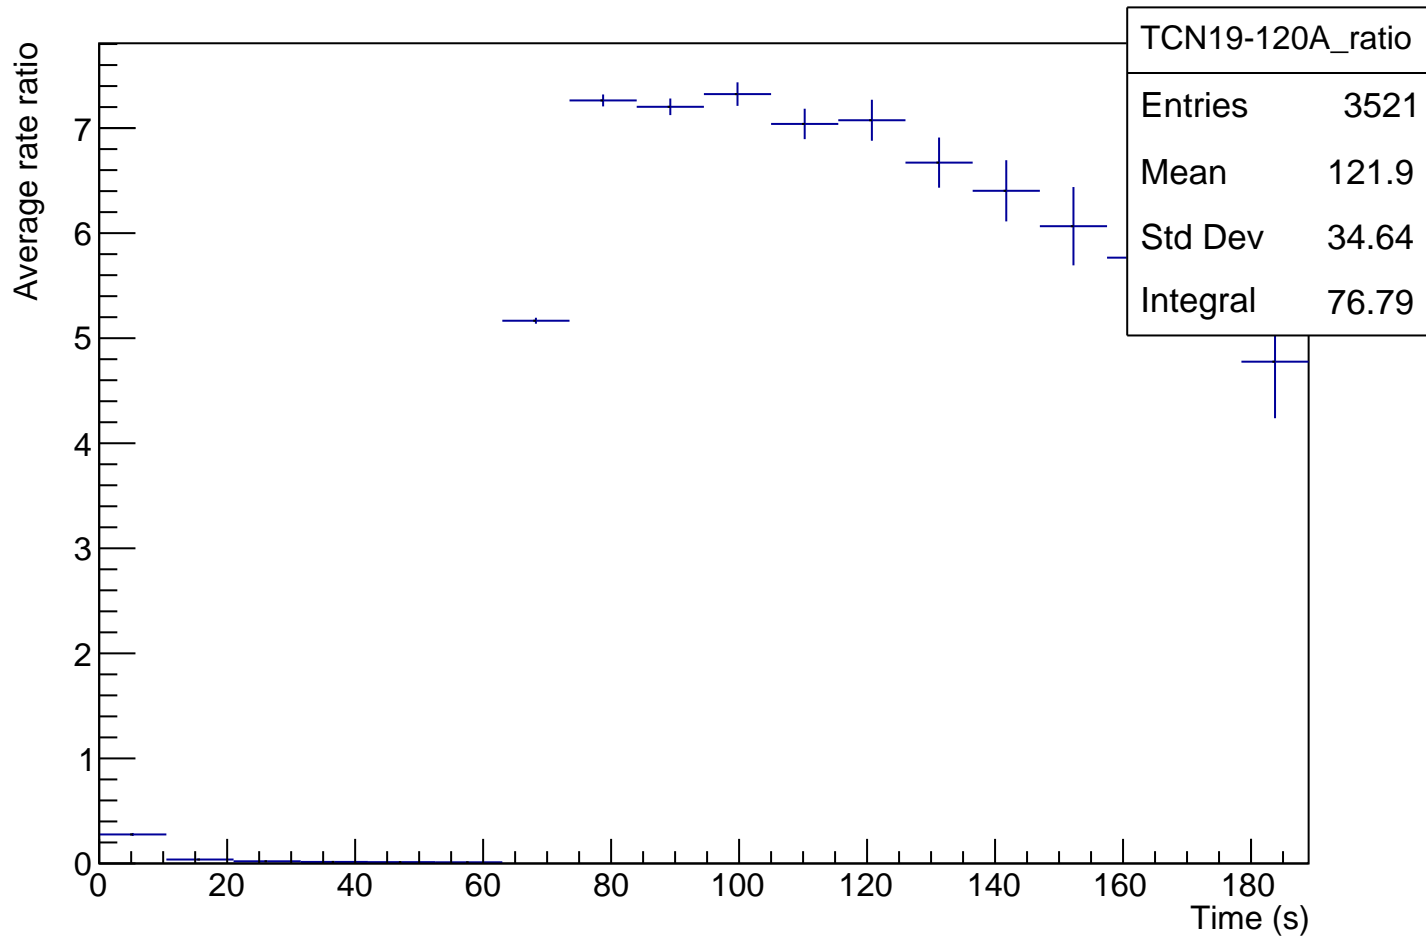

TCN19-120A

Count

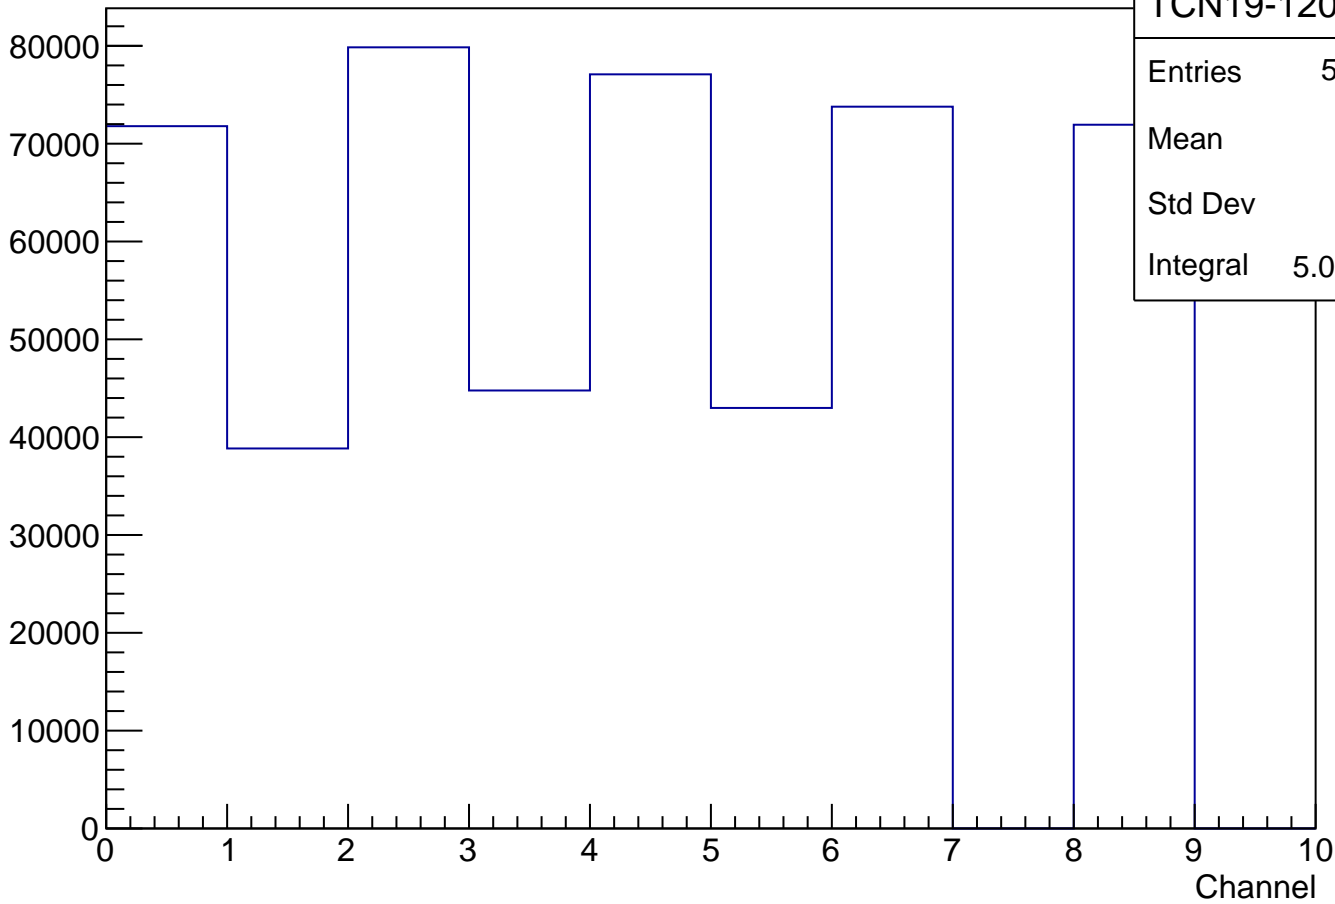

TCN19-120A_ch

Entries 501048


Mean 3.741

Std Dev 2.573

Integral 5.01e+05

Li6 window

Frequency

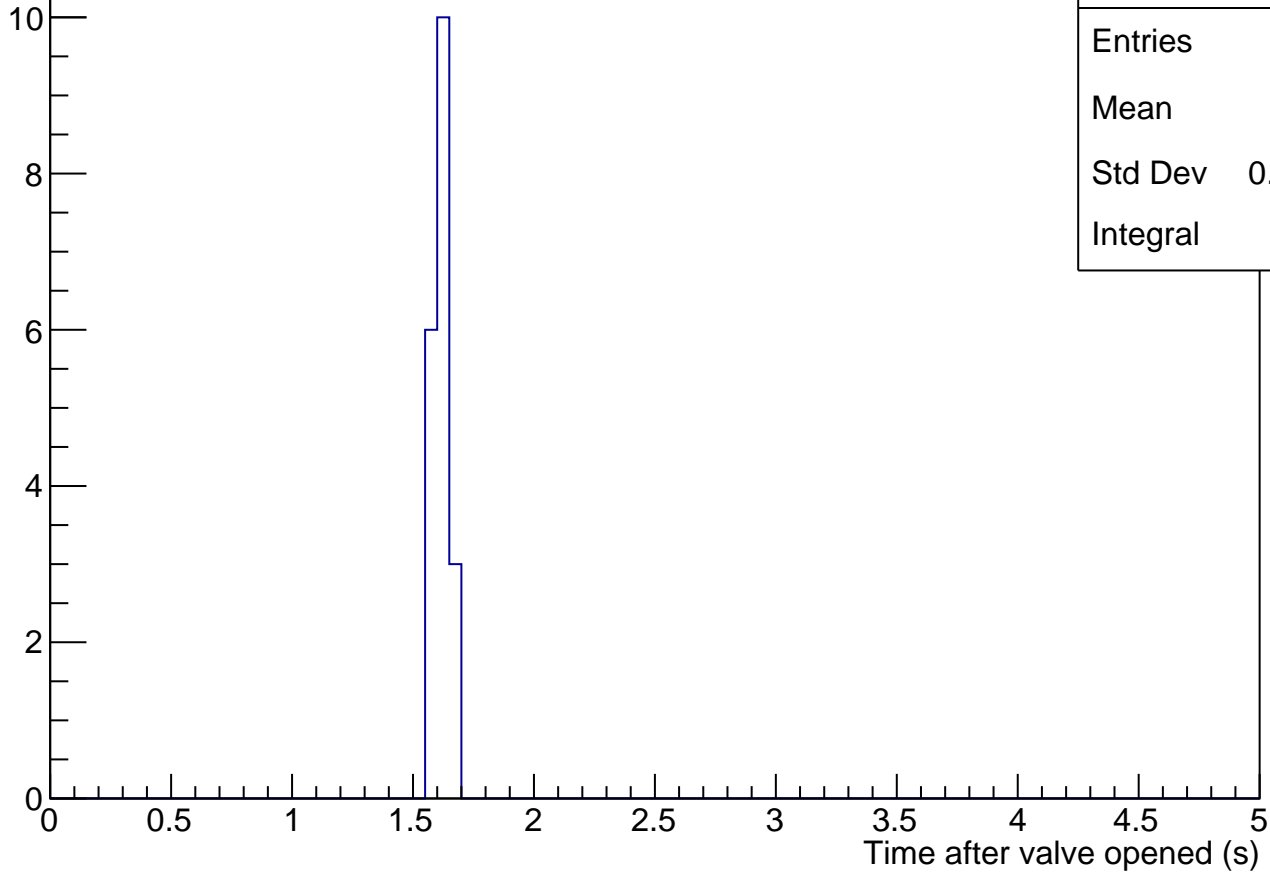

li6window

Entries 19

Mean 1.592

Std Dev 0.03349

Integral 19