


Fig S3 | Multi-instrument sensitivity analysis, and the estimator we excluded

a Weighted mode is not usable at this instrument count



b Why: the instrument count

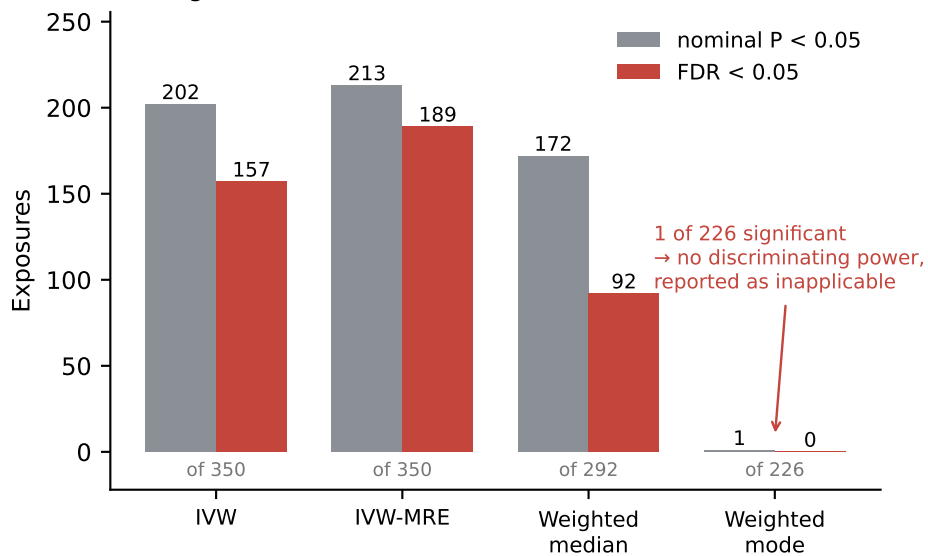