



313.15 K pressure fit and untouched concentration/source checks

○ Hilliard (validation) - - M2 - - M4 pressure fit ○ Hilliard (training) × Jou (validation)

17 wt% MEA
validation

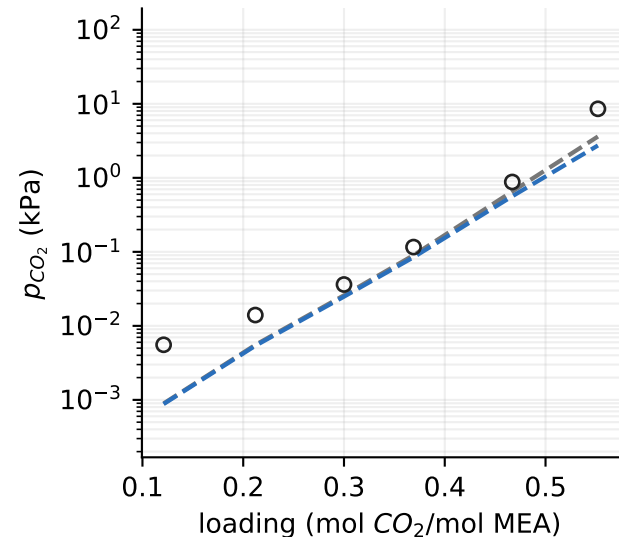

30 wt% MEA
training + Jou validation

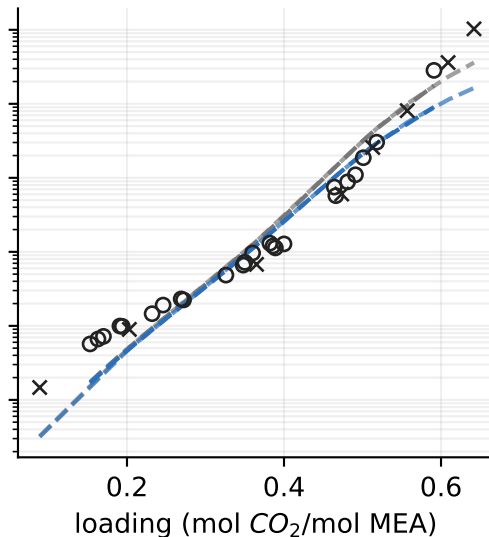

40 wt% MEA
validation

