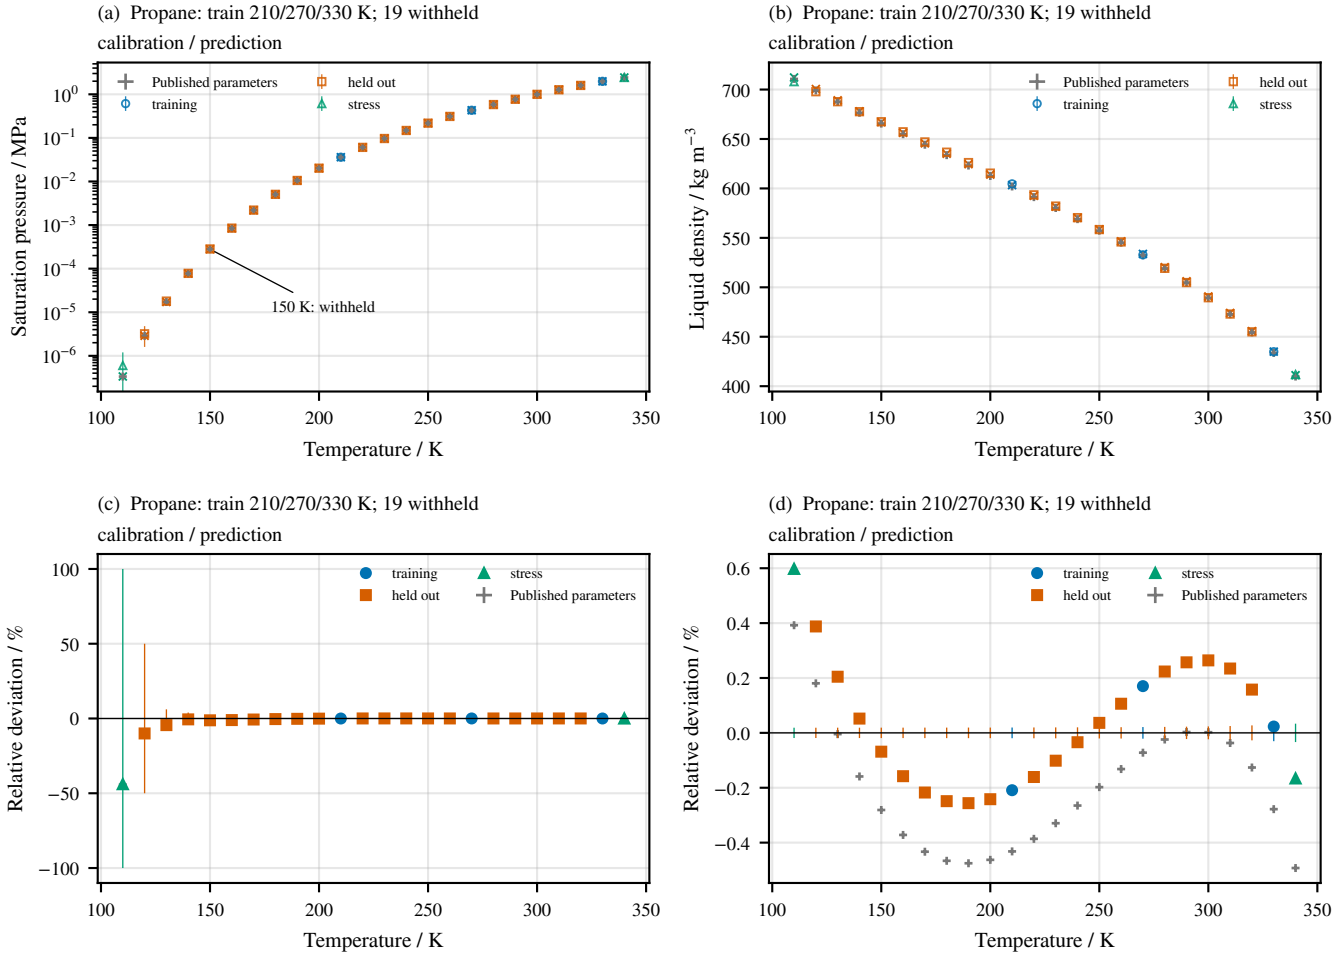

Top: measurements and discrete model values. Middle: relative deviations. Bottom: chloride calibration errors.