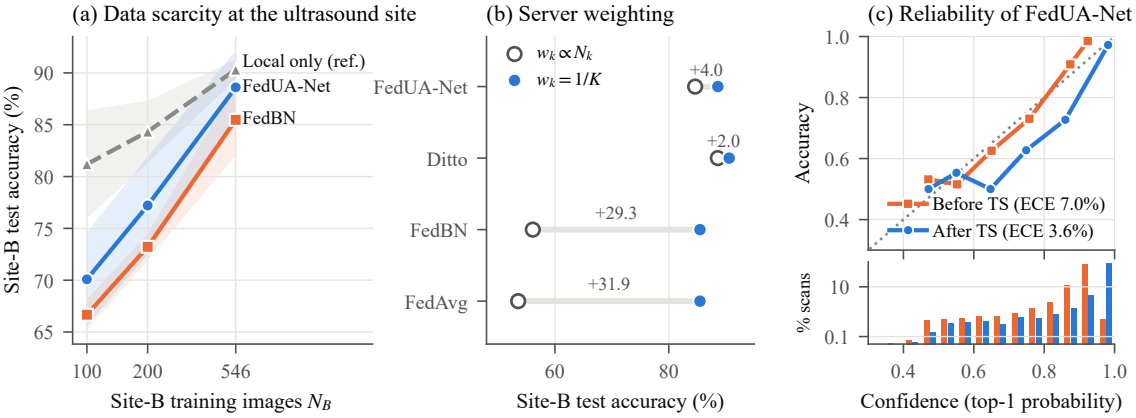
(a) Data scarcity at the ultrasound site
Site-B test accuracy (%)
90
85
80
75
70
65
Local only (ref.)
FedUA-Net
FedBN
100
200
546
Site-B training images N_B
(b) Server weighting
$w_k \propto N_k$
$w_k = 1/K$
FedUA-Net
Ditto
FedBN
FedAvg
+4.0
+2.0
+29.3
+31.9
60
80
Site-B test accuracy (%)
(c) Reliability of FedUA-Net
Accuracy
1.0
0.8
0.6
0.4
Before TS (ECE 7.0%)
After TS (ECE 3.6%)
% scans
10
0.1
0.4
0.6
0.8
1.0
Confidence (top-1 probability)