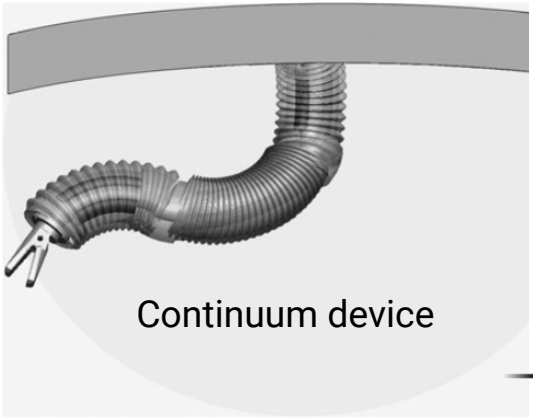
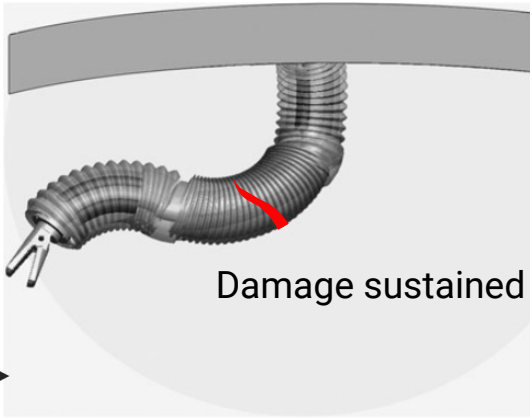
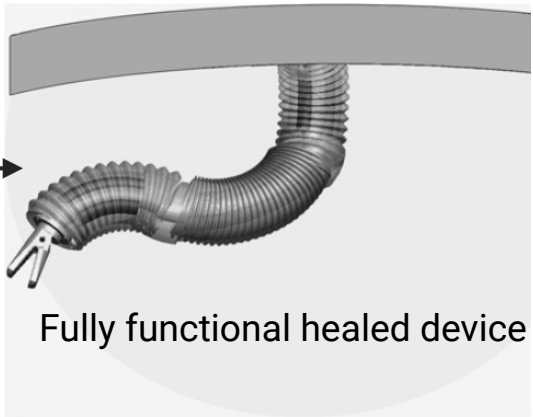

Continuum device


Damage sustained


Healing time


Fully functional healed device