

2, SIIEC Workspace, Basic Engineering Laboratory, SRM IST, Kattankulathur, Chengalpattu Dt., Tamil Nadu, India-603203.


CIN: U72900TN2022PTC154507

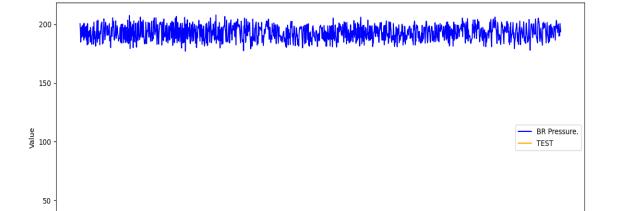

Combined Sensor Data - 01-10-2024 to 02-10-2024

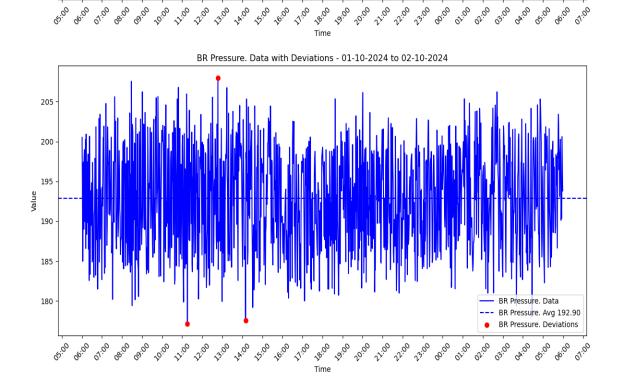

2, SIIEC Workspace, Basic Engineering Laboratory, SRM IST, Kattankulathur, Chengalpattu Dt., Tamil Nadu, India-603203. CIN: U72900TN2022PTC154507

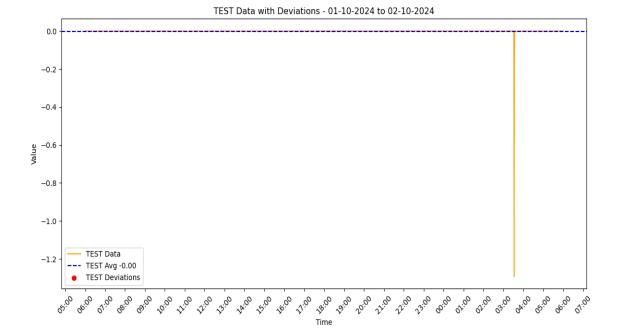

Sensor	Min Value	Max Value	Average Value	Mean Value	Median Value	No. Deviations
BR Pressure.	177.18	207.96	192.90	192.90	193.12	3
TEST	-1.29	0.00	-0.00	-0.00	0.00	0