


MEASUREMENTS

Module mmWave V4.0 Built for 5G-Advanced Ready for 6G!

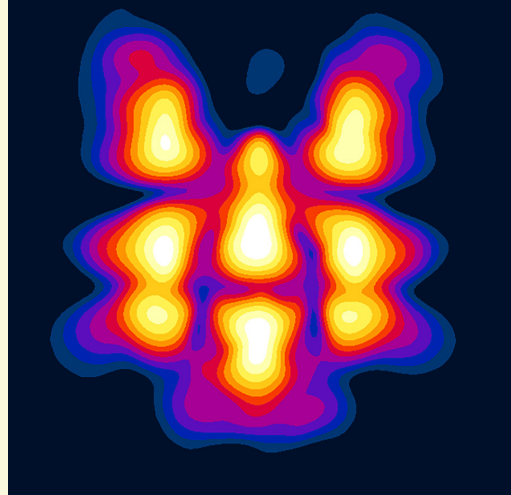

Accurate Closest Near-Field IPD Evaluations


IT'IS has achieved a breakthrough in assessment of closest near-field incident power density (IPD), and SPEAG has implemented the discovery with its release of [DASY8 Module mmWave V4.0](#). The latest version delivers faster, more accurate equivalent source reconstruction, Multi-TX exposure analysis, and more than 5,000 new 5G new radio (5G NR) and Wi-Fi 7 signals – ready for 5G-Advanced and 6G FR3!

Automated SAR Reporting with DASY8




SPEAG's new [DASY8 Report Assistant](#) automates specific absorption rate (SAR) reporting, generating customized Word reports and Excel summaries directly from DASY8 measurement data. Reusable templates help reduce manual effort, improve consistency, and minimize reporting errors.

Module SENS V2.0 Phantom Package PP4SENSV1 *Advancing Use-Case Testing*

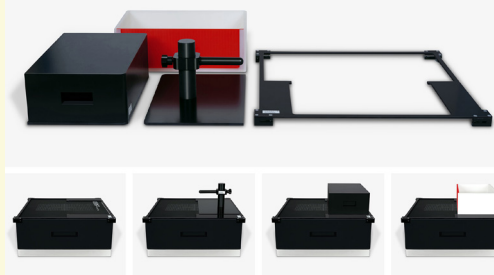

SPEAG has introduced [PP4SENSV1](#), a new phantom package for proximity sensor testing with DASY8 Module SENS. The package combines three specialized phantoms and a positioning frame to enable accurate, repeatable testing across different sensor technologies, materials, and use cases.

cSAR3D >1000-Sensor Array Verification in Seconds

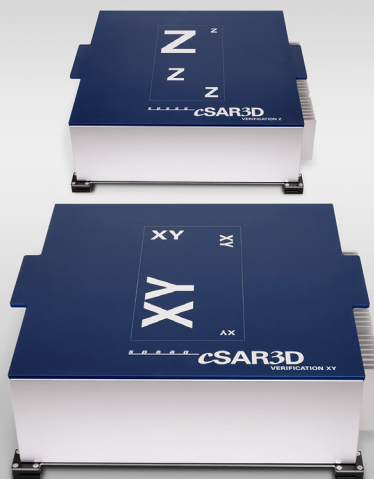

Comprehensive Sensor Verification Solved

SPEAG has introduced a new cSAR3D Verification Device for rapid sensor verification. The active device components, which are fully integrated with the upcoming cSAR3D V6.0 software, enable fully automated verification checks with clear pass/fail results. The new device helps laboratories and production environments increase efficiency while ensuring reliable measurements. Find out [more](#).

WORKSHOPS

Workshop Highlights Across Asia

The Z43 workshops in Taiwan, China, and Korea organized by AUDEN, DYMSTEC, and TUOPUMED, provided a great opportunity to share updates, exchange ideas and experiences, and engage with our customers, researchers, and industry experts. A big thank you to everyone involved!



TEMPORAL INTERFERENCE


Advanced GUI for Clinical Studies with TIBS-R



TI Solutions and the IT'IS Foundation offer custom graphical user interface (GUI) development for TIBS-R, tailored to study-specific workflows and designed to simplify operation in clinical settings. Read more about it [here](#).

Improved Synchronization and Control for TIBS-R

With the latest [TIBS-R firmware V3.4](#), TI Solutions introduces enhanced trigger and synchronization options, simpler protocol programming, and configurable voltage limits. These updates provide greater flexibility and control for integration of external devices and for running advanced stimulation protocols.

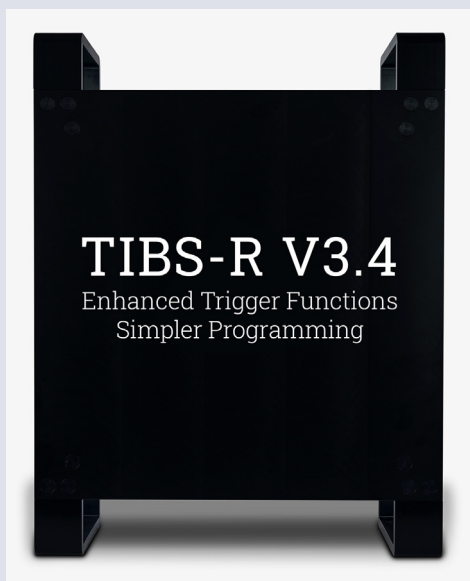

VIRTUAL POPULATION



New Pediatric Model

[THALIA V1.0](#) is now hosted in the IT'IS Virtual Population library. Developed by researchers at the Athinoula A. Martinos Center for Biomedical Imaging at Massachusetts General Hospital and Harvard Medical School, in collaboration with colleagues from EPFL and Boston Children's Hospital, the high-resolution model represents the anatomy of a 10-month-old girl across 442 segmented tissue compartments. Congratulations on this achievement!

EDUCATION



Bachelor's, Master's, and PhD students: Got a Sim4Life project worth showing off? [Submit](#) your simulation file for an original Sim4Life project or from a 2026 paper or presentation to compete for prizes of USD 3,000, 2,000, and 1,000. Entries close 31 October 2026!

EVENTS



Z43 Summer Night Party

The weather had other plans for our Summer Night Party, but we did not let a little bit of rain stop the celebration! From the first drink to the last conversation, it was an evening full of good food, plenty of laughs, and great company. Thanks to everyone who joined us!

RESEARCH

PUBLICATIONS

Enhancement of Sleep Slow Wave Activity using Transcranial Electrical Stimulation with Temporal Interference: An Interim Analysis of the STRENGTHEN Study

L. Schaeffer, *et al.*, 2026, Communications Medicine, doi: [10.1038/s43856-026-01744-x](#) (online 01 July 2026)

Biodegradable Smart Face Mask for Cough Acoustic Sensing

M. J. Bathaei, *et al.*, 2026, ACS Sensors, doi: [10.1021/acssensors.5c04572](#) (online 09 July 2026)

Accelerating the Development of Bioelectronic Medicine: Outcomes and Innovations from the NIH SPARC Initiative

B. Patel, *et al.*, 2026, Bioelectronic Medicine, doi: [10.1186/s42234-026-00213-z](#) (online 04 September 2026)

A Generalized Activating Function for Rapid and Accurate Neural Response Prediction in Spinal Cord Stimulation

T. H. Newton, *et al.*, 2026, Communications Biology, doi: [10.1038/s42003-026-10849-x](#) (online 08 September 2026)

Information Content and Interpretation of CSD Non-trivially Depends on Array Density

J. J. Tharayil, *et al.*, 2026, Journal of Neural Engineering, doi: [10.1088/1741-2552/ae93f9](#) (online 15 September 2026)