iKey Medical




DeltaWay

Femoral Stem

iKey Medical CopyRight © 2024

12/14 Taper

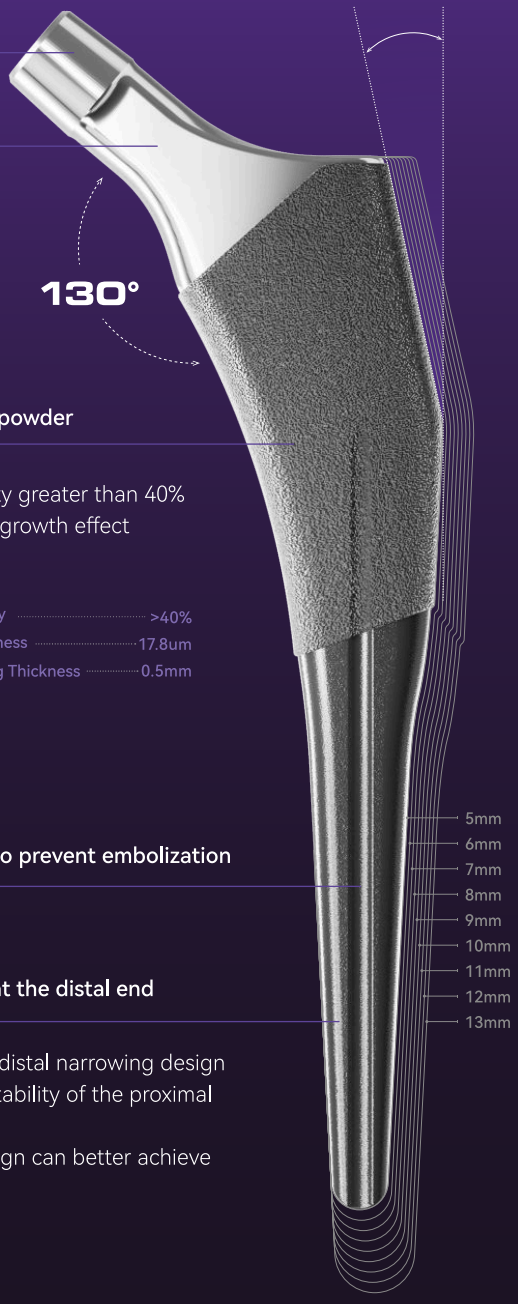

Imported pure titanium powder vacuum spraying

Thickness 0.5mm, porosity greater than 40%
Provide excellent bone ingrowth effect



Porosity	>40%
Roughness	17.8um
Coating Thickness	0.5mm

Decompression groove to prevent embolization

Porous coating surface at the distal end

Smooth transition of the distal narrowing design
Strengthen the fixation stability of the proximal coating area
The distal narrowing design can better achieve proximal matching

12° wedge shape design
Lowerrisk of greater trochanter fractures during surgery





- The small A/P diameter preserves bone mass while providing good torsional stability
- The flat design of the A/P position reduces the risk of fracture during surgery



Proximal
Tight fit of the proximal end and cancellous bone


Upper Middle
The middle and upper parts are in close contact to the anterior femoral cortex

Upper Distal
The mid-distal part is in close contact to the posterior femoral cortex

Three parts jointly ensure that the stem is well locked on the correct line of force in the medullary cavity

Complete specifications and models to achieve better medullary cavity matching

Part Code	Specification	Stem Length A(mm)	Offset B(mm)	Neck Length C(mm)	Distal Dia D(mm)
A216418	0# STD 12/14	130	36	32.5	5
A216419	1# STD 12/14	132	36.5	32.5	6
A216420	2# STD 12/14	134	37	32.5	7
A216421	3# STD 12/14	136	37.5	32.5	8
A216422	4# STD 12/14	137	38	32.5	8
A216423	5# STD 12/14	140	38.5	32.5	8
A216424	6# STD 12/14	142	39	32.5	9
A216425	7# STD 12/14	144	39.5	32.5	10
A216426	8# STD 12/14	146	40	32.5	11
A216427	9# STD 12/14	148	41	32.5	11
A216428	10# STD 12/14	150	42	32.5	12
A216429	11# STD 12/14	152	43	32.5	13

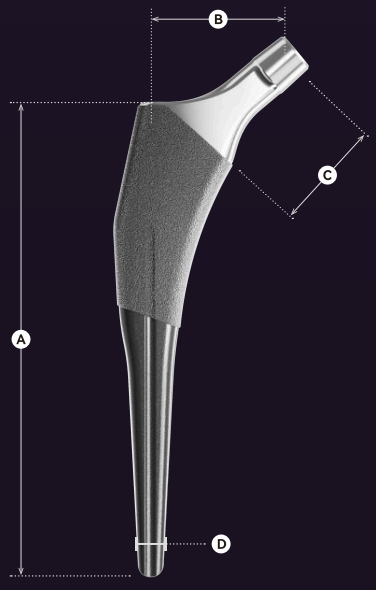

30 Yongchang South Road, Beijing Economic Technological Development Area,100176 Beijing,China.

Beijing iKey Medical Device Tecthnology Co.,Ltd. | 010-67850177-8001 | sales@ikey-medical.com