


Ion Chamber Measurement Data

System Information	
Procedure Date:	12/8/2023
Tube Model:	DT-1084
Tube Serial:	10277-01
Tube kV:	120 kV
Beam Quality:	120-M
Generator Model:	X-4119
Generator Serial:	A013468

Reference Dosimeter Information	
Ion Chamber ID:	RAD-008
Manufacture:	RadCal
Ion Chamber Model:	10x0.6-6
Ion Chamber Serial:	02-1964
Digitizer Model:	ADDM+
Digitizer Serial:	47-1995
Calibration Due Date:	1/24/2024

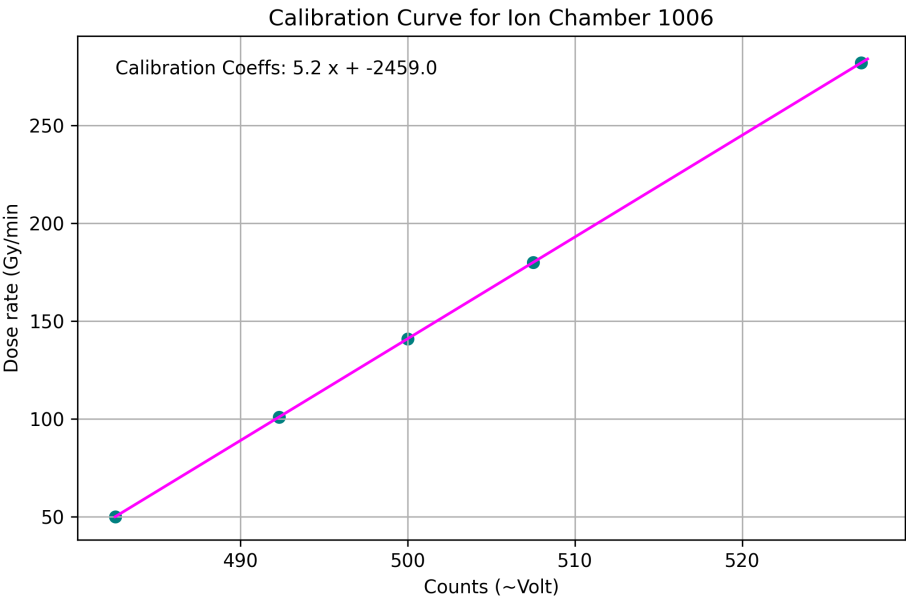

Ionization Chamber Information:

Model: Type J
 Serial: 1006

Digitizer/Electrometer Information:

Model: Phantom C Daughter Card
 Serial: 1014
 Scale: Dose Rate
 Range: Gy/min

Calibration Coeffs	
System Coeff (Gy/min/Rdg):	5.200
System Offset (Gy/min):	-2459.000
System Uncertainty:	N/A

Environmental Conditions: T=22.1 °C, P=99.58 kPa, RH=34%

Calibrated By:
 Jacob Garner, B.S.
 Calibration Technician

Reviewed By:
 Physicist or Calibration Lab
 Committee Member or Dsignee