


Ion Chamber Measurement Data

| System Information | |
|--------------------|-----------|
| Procedure Date: | 12/8/2023 |
| Tube Model: | DT-1084 |
| Tube Serial: | 10277-01 |
| Tube kV: | 120 kV |
| Beam Quality: | 120-M |
| Generator Model: | X-4119 |
| Generator Serial: | A013468 |

| Reference Dosimeter Information | |
|---------------------------------|-----------|
| Ion Chamber ID: | RAD-008 |
| Manufacture: | RadCal |
| Ion Chamber Model: | 10x0.6-6 |
| Ion Chamber Serial: | 02-1964 |
| Digitizer Model: | ADDM+ |
| Digitizer Serial: | 47-1995 |
| Calibration Due Date: | 1/24/2024 |

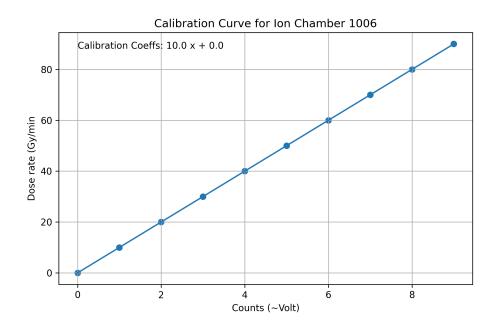

Ionization Chamber Information:

Model: Type J Serial: 1006

Environmental Conditions: T=22.1 °C, P=99.58 kPa, RH=34%

Calibrated By:

Jacob Garner, B.S. Calibration Technician Reviewed By:
Physicist or Calibration Lab
Committee Member or Dsignee