


In-vitro finite-time response: threshold-triggered stochastic passage

C01 and C02; initial 2N-6N; five fixed p_misseg values; oxygen 0-20%; time 0-10,000 days

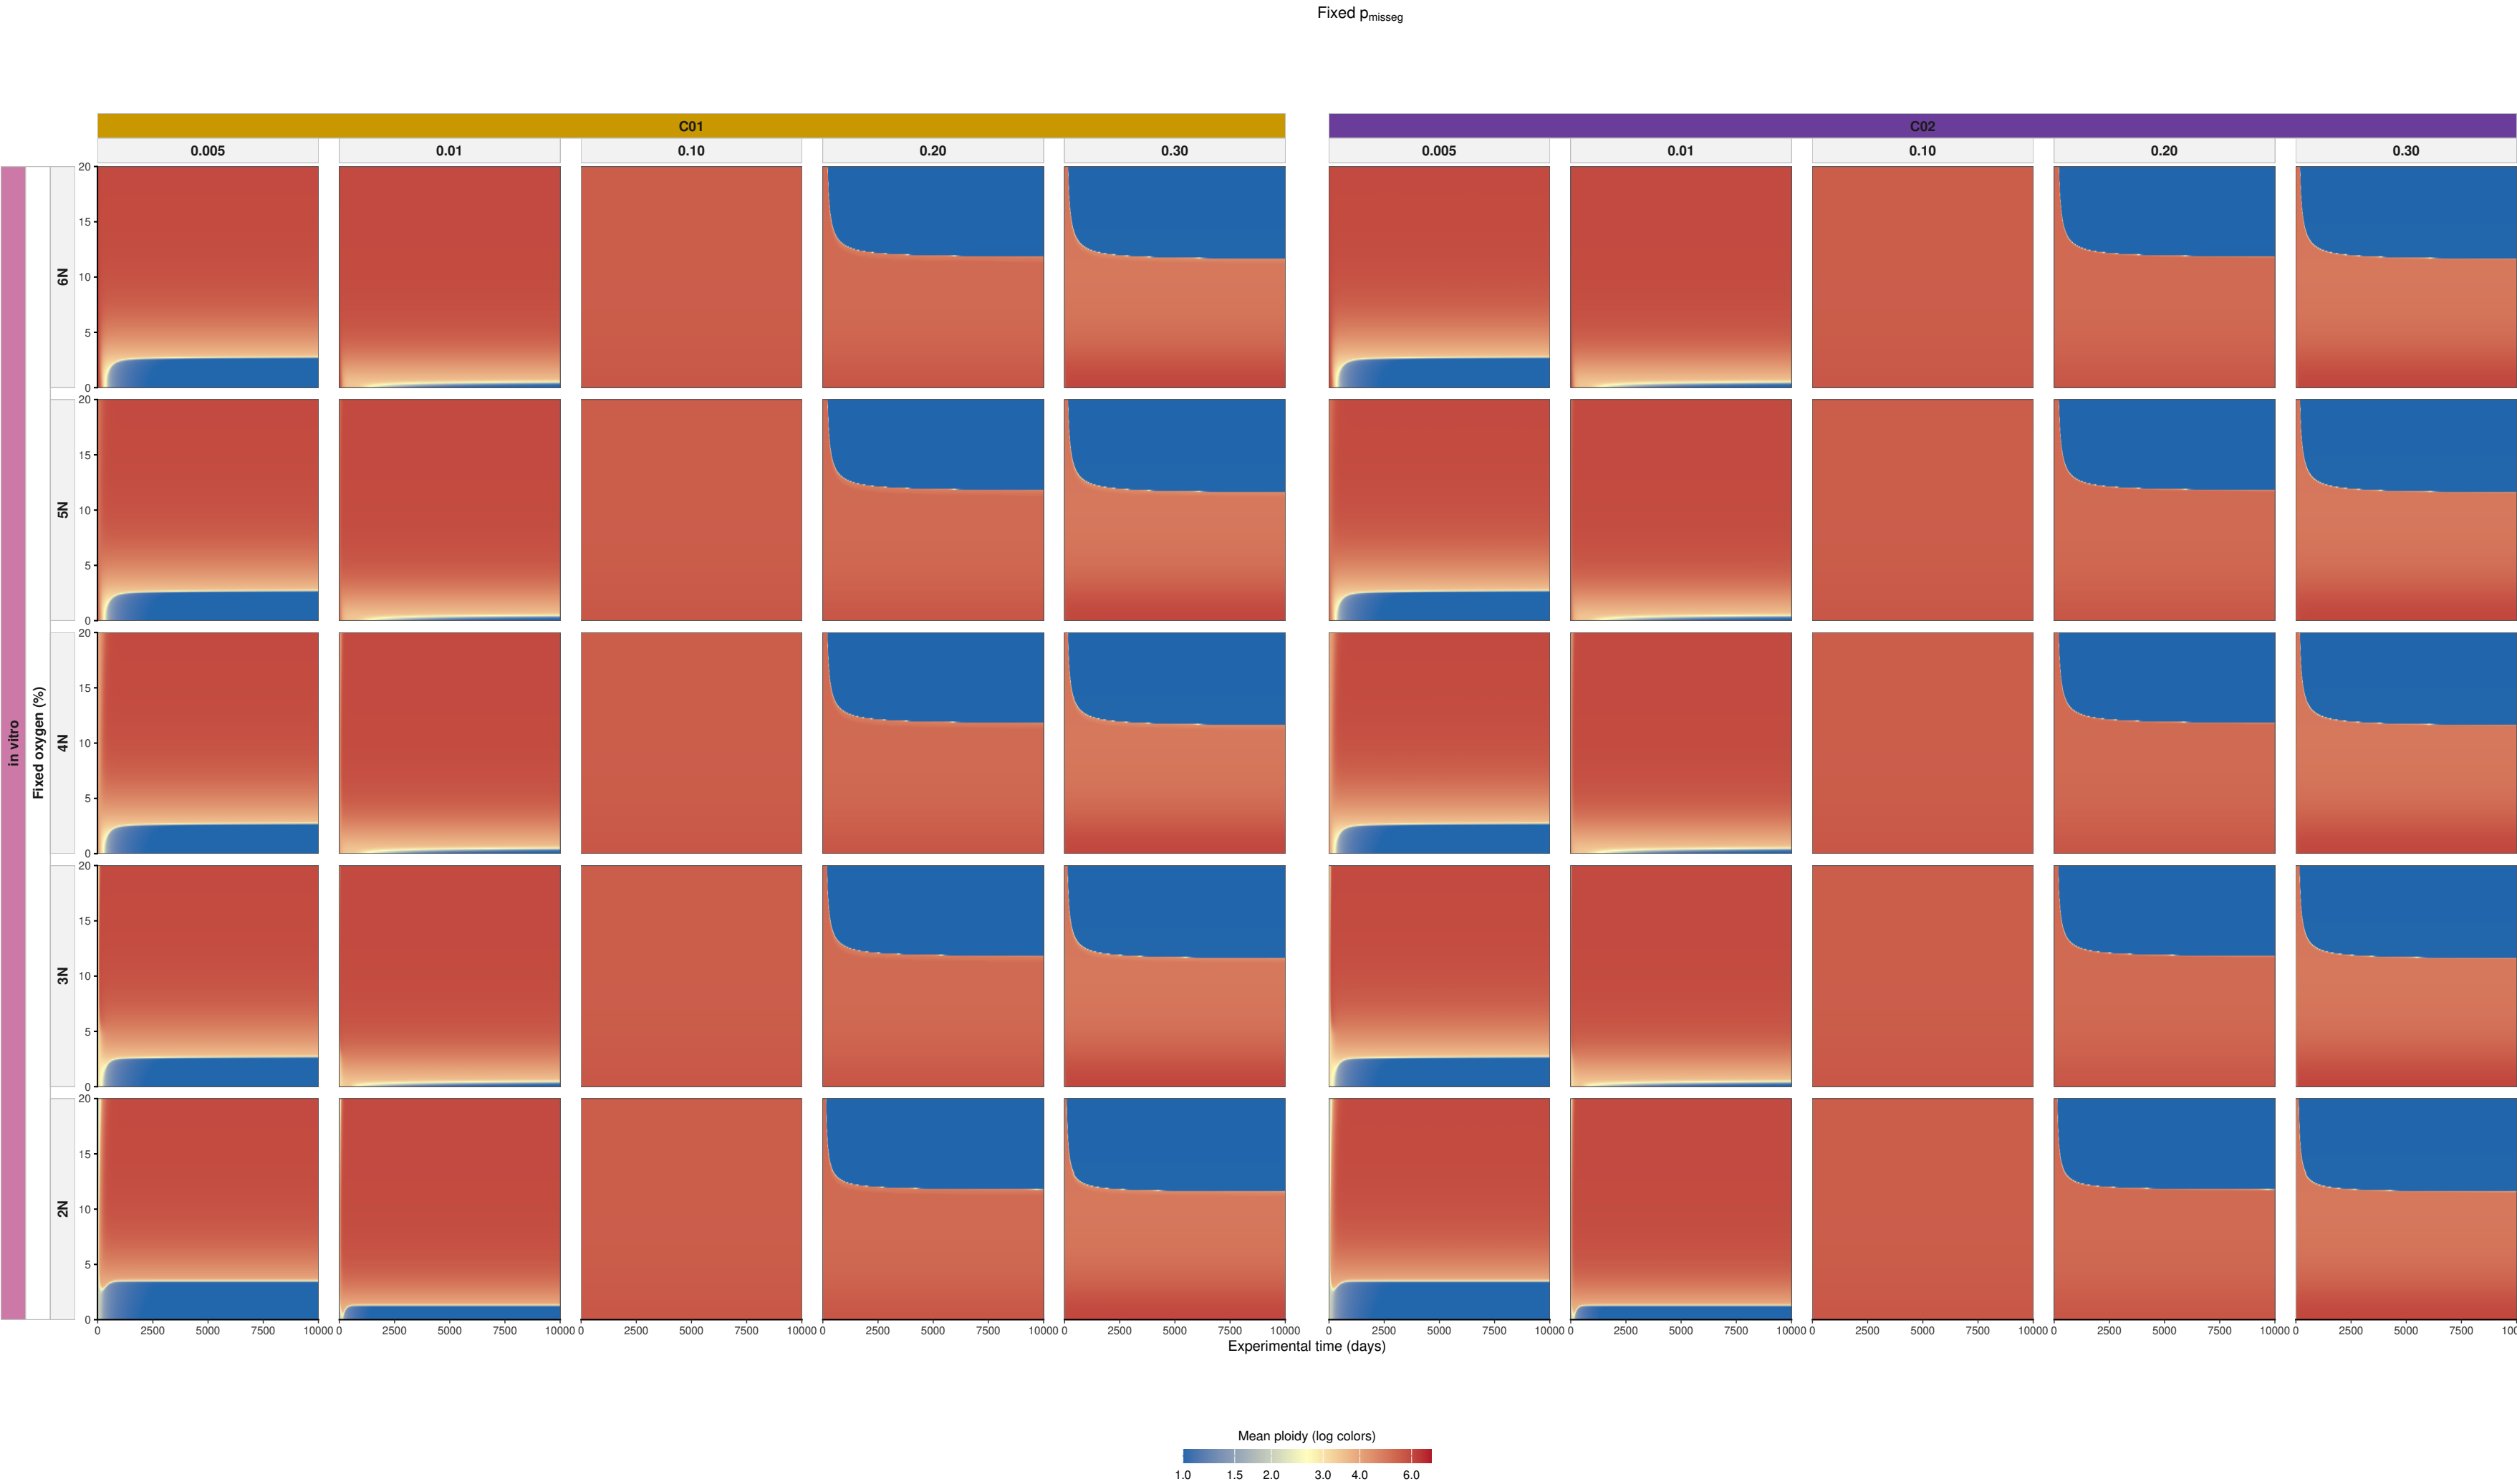

Full stored data use daily values from 0 to 10,000 days; the diagnostic raster displays every 20th day at the full oxygen grid. Passage is triggered on the first eligible integer day; sampling uses that day's actual population. Means include all 50 endpoints.