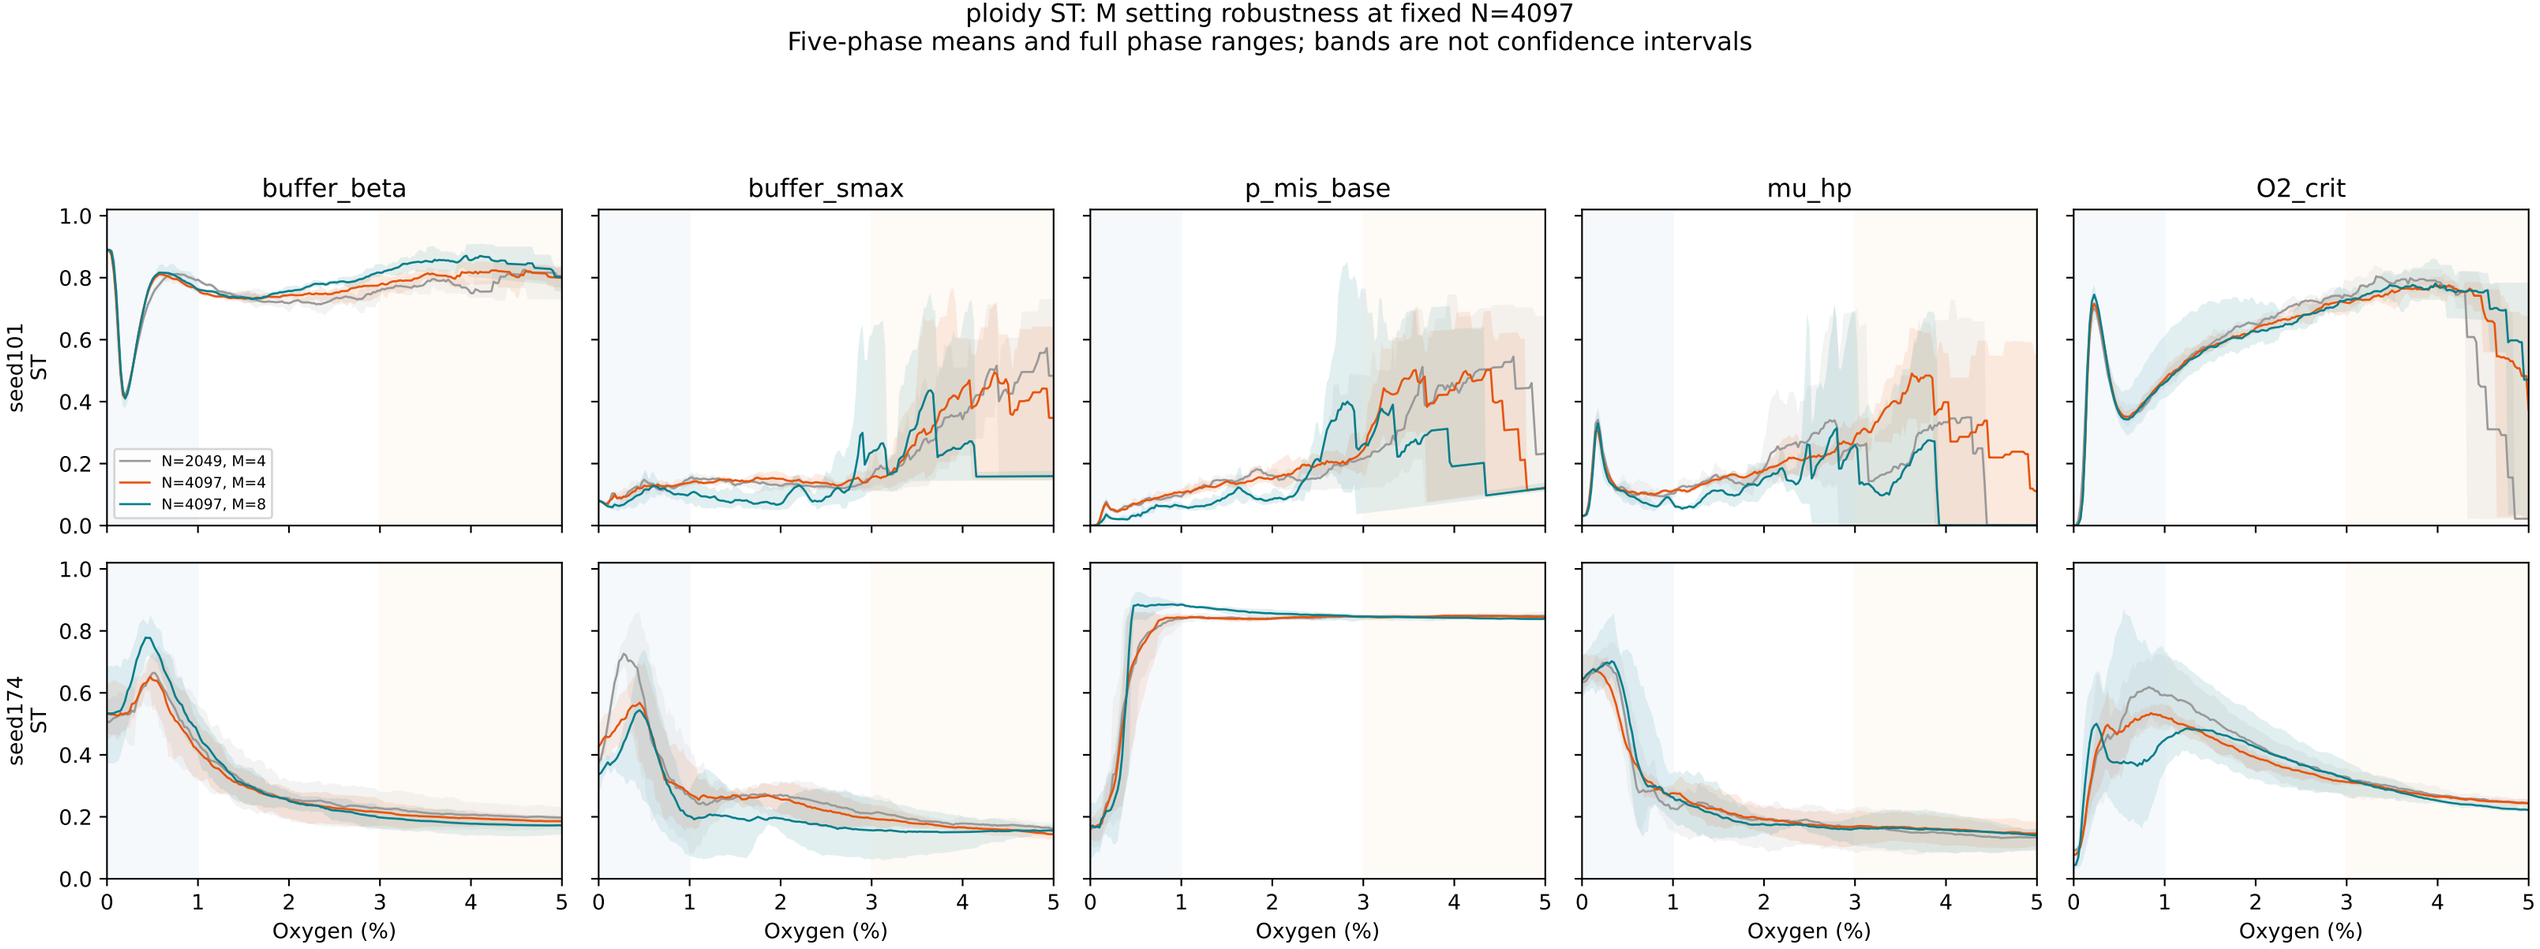

ploidy ST: M setting robustness at fixed N=4097
Five-phase means and full phase ranges; bands are not confidence intervals
buffer_beta
buffer_smax
p_mis_base
mu_hp
O2_crit
seed101 ST
seed174 ST
N=2049, M=4
N=4097, M=4
N=4097, M=8
0.0
0.2
0.4
0.6
0.8
1.0
0
1
2
3
4
5
Oxygen (%)