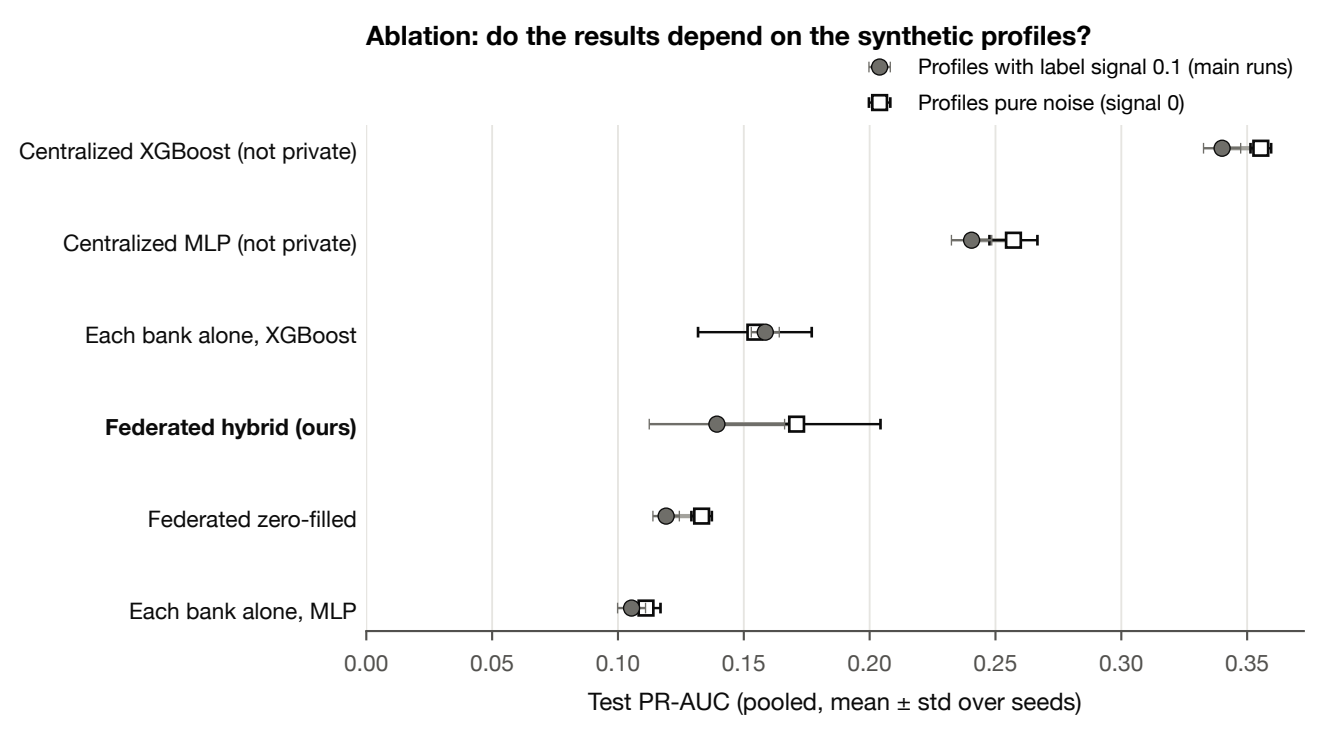
Ablation: do the results depend on the synthetic profiles?
Profiles with label signal 0.1 (main runs)
Profiles pure noise (signal 0)
Centralized XGBoost (not private)
Centralized MLP (not private)
Each bank alone, XGBoost
Federated hybrid (ours)
Federated zero-filled
Each bank alone, MLP
0.00
0.05
0.10
0.15
0.20
0.25
0.30
0.35
Test PR-AUC (pooled, mean ± std over seeds)