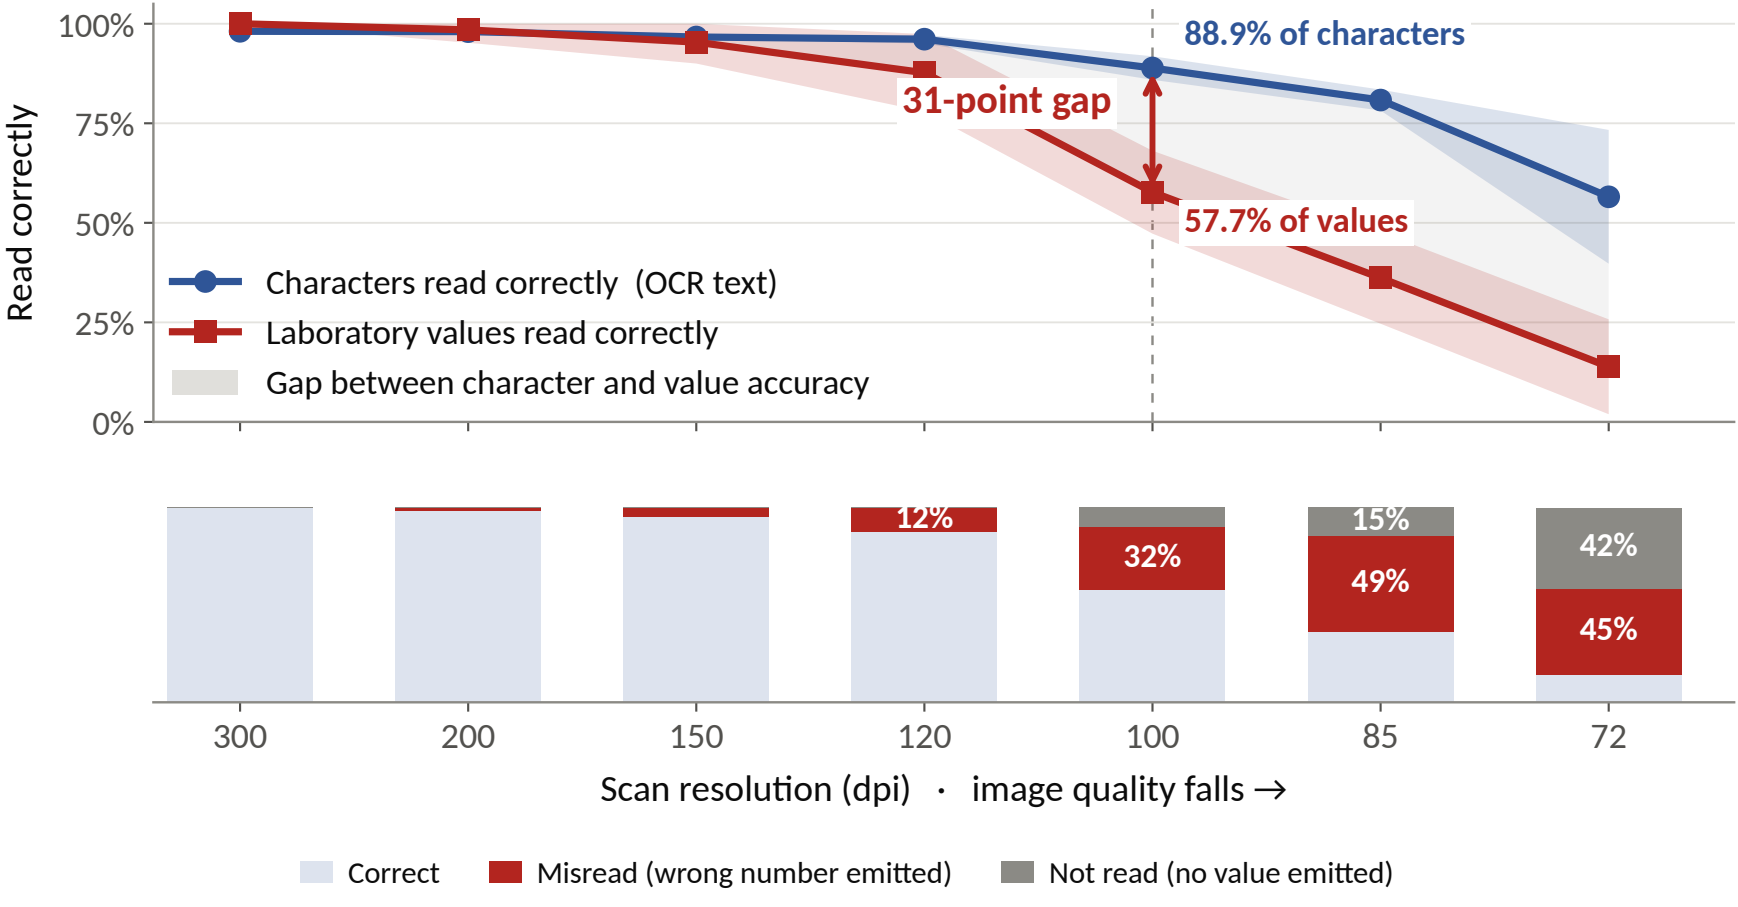
Read correctly
100%
75%
50%
25%
0%
88.9% of characters
31-point gap
57.7% of values
Characters read correctly (OCR text)
Laboratory values read correctly
Gap between character and value accuracy
12%
32%
15%
49%
42%
45%
300
200
150
120
100
85
72
Scan resolution (dpi) · image quality falls →
Correct
Misread (wrong number emitted)
Not read (no value emitted)