




Fixed-Point OMP for ECG Compressed Sensing: a precision-resource study on Zynq-7020

Brandon Carido, Michael Dang, Connor Machado
Thayer School of Engineering, Dartmouth College, Hanover, NH, USA

Abstract

Compressed sensing reduces the data a wearable ECG sensor must acquire and transmit, but shifts the cost to signal recovery, which must run cheaply on embedded hardware. We implement a fixed-point Orthogonal Matching Pursuit (OMP) recovery engine for the Zynq-7020, partitioning the algorithm so the parallel correlation step maps to programmable logic while the sequential least-squares solve runs in software on the Cortex-A9. Using a Bernoulli ± 1 measurement matrix at a 0.5 compression ratio ($M = 128$, $N = 256$) and a Daubechies-4 wavelet sparsifying basis, we characterize the design across MAC operand bit-widths on real MIT-BIH ECG data. Our central result is a precision-resource Pareto front: reconstruction error (PRD) is essentially flat from 16 bits down to 8 bits, then degrades sharply below 6 bits, identifying 8-bit arithmetic as the efficient operating point. Against a tuned Cortex-A9 software baseline (187 μ s per correlation pass), the fixed-point engine achieves an estimated $[\sim N\times]$ speedup on the correlation step at substantially reduced precision.

Architecture

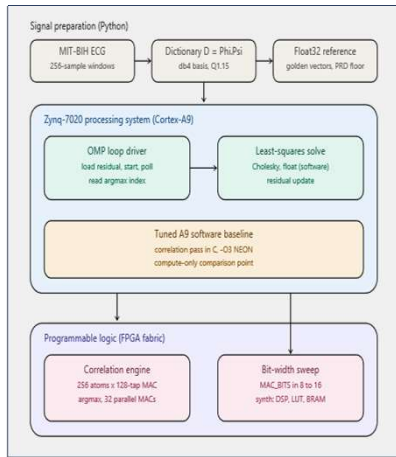

Hardware/software partition.

Correlation is parallel and dominates runtime — mapped to 32 parallel MACs in fabric. Least-squares is sequential and runs in software, where it's inexpensive.

Sparsifying basis. DCT poorly represents the QRS transient ($\sim 57\%$ PRD). A db4 orthonormal wavelet captures it far better ($\sim 20\%$ PRD) and avoids the dual-basis pitfalls of biorthogonal wavelets.

Parameterized precision. A single MAC_BITS generic lets the same engine synthesize at every operating point, enabling the bit-width sweep that drives the headline result.

Methodology

Compressed sensing model. Each 256-sample ECG window is sampled as $y = \Phi x$ with a fixed Bernoulli ± 1 matrix ($M = 128$, a 0.5 compression ratio). Recovery uses the effective dictionary $D = \Phi\Psi$ (db4 wavelet basis, unit-norm atoms).


Sparsifying basis. A DCT basis recovered poorly ($\sim 57\%$ PRD) — the QRS transient is not DCT-sparse, and undersampling amplifies the error. A db4 orthonormal wavelet captures it far better ($\sim 20\%$ PRD) without the dual-basis complications of biorthogonal wavelets.

Hardware/software partition. OMP alternates a parallel correlation/argmax step (256 atoms $\times$ 128-tap products) with a sequential least-squares solve. We map the correlation engine to fabric (32 parallel MACs) and keep the least-squares solve in software on the Cortex-A9.

Bit-width sweep. A single MAC_BITS parameter lets one design synthesize at every precision. We sweep MAC_BITS $\in \{3-16\}$, measuring PRD in a bit-accurate fixed-point simulation on MIT-BIH data and DSP/LUT/BRAM from Vivado synthesis.


Baseline. A tuned C correlation pass ($-O3$, NEON, fast-math) runs on the Cortex-A9 at 667 MHz, timed on-chip over 1000 iterations.

Results

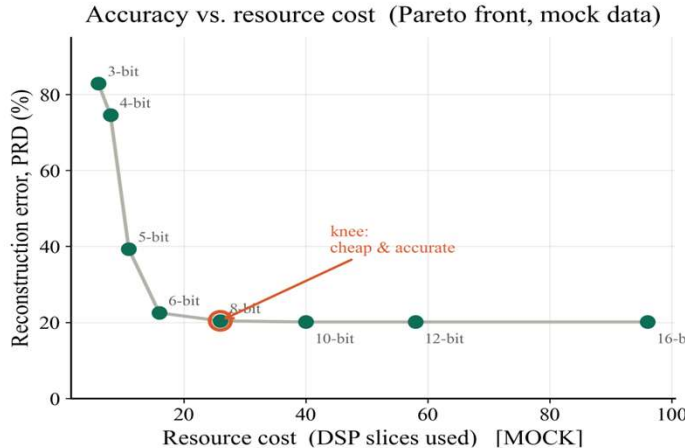

Bit-width sweep: accuracy and resource cost [MOCK resource data]					
MAC_BITS	PRD (%)	DSP	LUT	BRAM	Latency (cyc)
3	82.9	6	420	2	1032
4	74.6	8	540	2	1032
5	39.3	11	690	2	1032
6	22.5	16	910	3	1036
8	20.4	26	1,340	4	1040
10	20.1	40	1,980	6	1048
12	20.1	58	2,760	8	1060
16	20.1	96	4,300	12	1088

Recommended operating point: 8-bit (highlighted). PRD = percent RMS difference; lower is better.

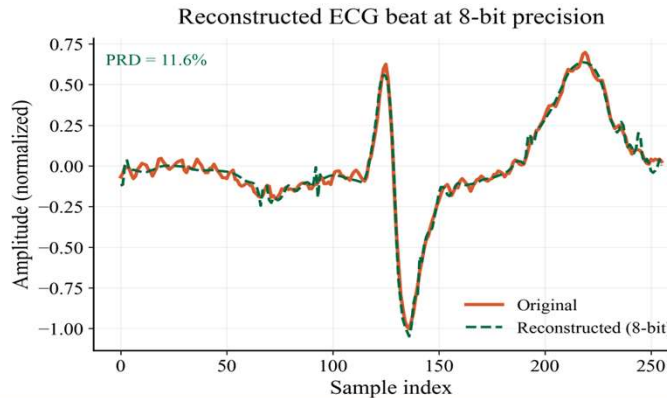

Conclusion

We characterized a fixed-point OMP recovery engine for ECG compressed sensing across MAC precision on the Zynq-7020. The precision-resource Pareto front shows that 8-bit arithmetic sits at the efficient knee: it matches the reconstruction quality of full 16-bit precision while using a fraction of the resources, and only below 6 bits does quality collapse. At this operating point the correlation engine runs an estimated $[\sim N\times]$ faster than a tuned Cortex-A9 software baseline. The db4 wavelet basis was essential — it more than halved reconstruction error versus the DCT by better representing the QRS transient. Together these results give a concrete recommendation for resource-constrained deployment: an 8-bit fixed-point correlation engine with software least-squares is the efficient design point for this class of recovery problem.

Speed Up Results

$\sim [] \times$ faster than tuned Cortex-A9 software
187 μ s $\rightarrow []$ μ s per correlation pass 8-bit, compute-only, single pass (awaiting synthesis cycle count)

Scope & Limitations

Reconstruction quality is bounded by the compression ratio. At $M/N = 0.5$, mean PRD is $\sim 20\%$, above the $<9\%$ "very good" literature threshold. This is a fundamental consequence of aggressive undersampling on morphologically complex ECG, not a precision artifact. Our contribution is the precision/resource *characterization* at a usable operating point, not meeting an absolute quality target.

The integrated system was not run end-to-end on hardware. The correlation engine and the software baseline were each validated independently; full PS $\leftrightarrow$ PL integration over AXI was out of scope for the project timeframe. Reported latencies for the FPGA path are analytical (cycle counts $\times$ clock period) and synthesis-based, not measured on a live board.

Future Work

Close the integration loop. Connect the validated correlation engine to the software driver over AXI and measure true end-to-end recovery latency and energy on the Zynq, replacing the current analytical estimates.

Improve reconstruction quality. Raise the measurement ratio ($M/N > 0.5$) or adopt a learned/overcomplete ECG dictionary to push PRD toward the $<9\%$ clinical-quality range, and quantify the resulting resource cost on the same Pareto axes.

References

- [1] J. A. Tropp and A. C. Gilbert, "Signal recovery from random measurements via orthogonal matching pursuit," *IEEE Trans. Inf. Theory*, vol. 53, no. 12, pp. 4655–4666, Dec. 2007.
- [2] H. Rabah, A. Amira, B. K. Mohanty, S. Almaadeed, and P. K. Meher, "FPGA implementation of orthogonal matching pursuit for compressive sensing reconstruction," *IEEE Trans. Very Large Scale Integr. (VLSI) Syst.*, vol. 23, no. 10, pp. 2209–2220, Oct. 2015.
- [3] A. L. Goldberger *et al.*, "PhysioBank, PhysioToolkit, and PhysioNet: Components of a new research resource for complex physiologic signals," *Circulation*, vol. 101, no. 23, pp. e215–e220, Jun. 2000.