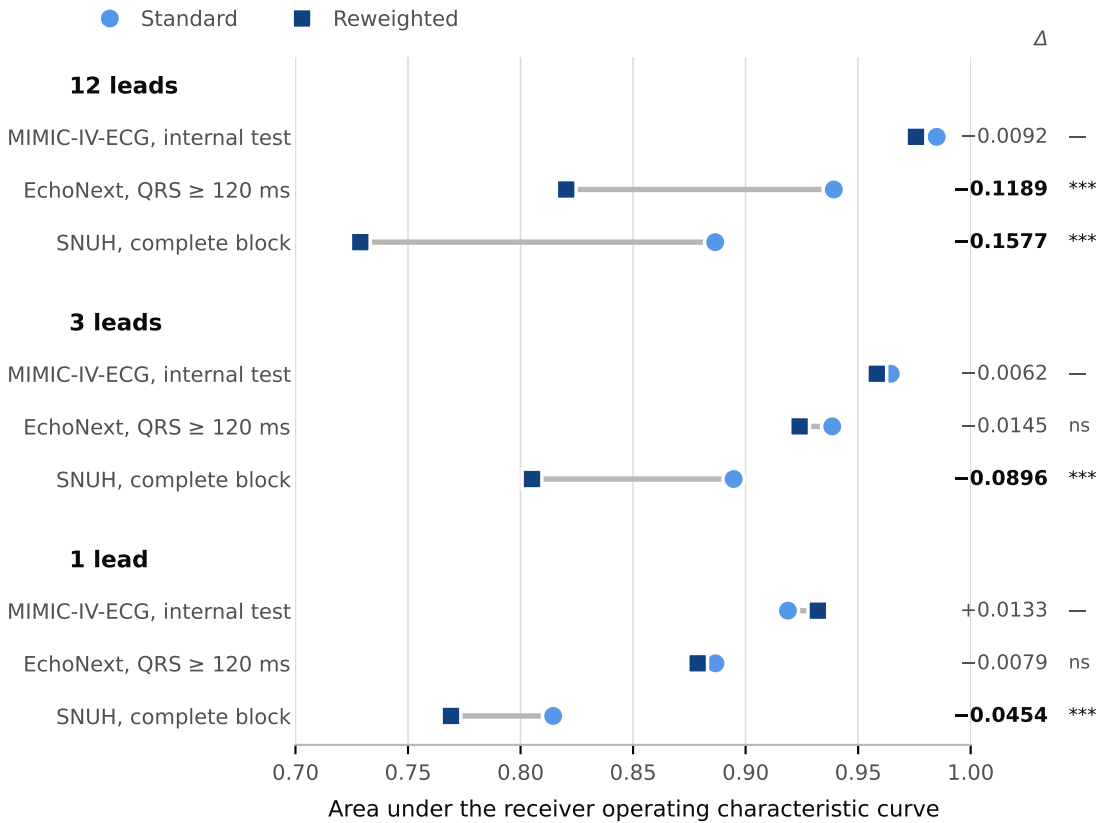
Standard
Reweighted
Δ
12 leads
MIMIC-IV-ECG, internal test
−0.0092
—
EchoNext, QRS ≥ 120 ms
−0.1189
***
SNUH, complete block
−0.1577
***
3 leads
MIMIC-IV-ECG, internal test
−0.0062
—
EchoNext, QRS ≥ 120 ms
−0.0145
ns
SNUH, complete block
−0.0896
***
1 lead
MIMIC-IV-ECG, internal test
+0.0133
—
EchoNext, QRS ≥ 120 ms
−0.0079
ns
SNUH, complete block
−0.0454
***
0.70
0.75
0.80
0.85
0.90
0.95
1.00
Area under the receiver operating characteristic curve