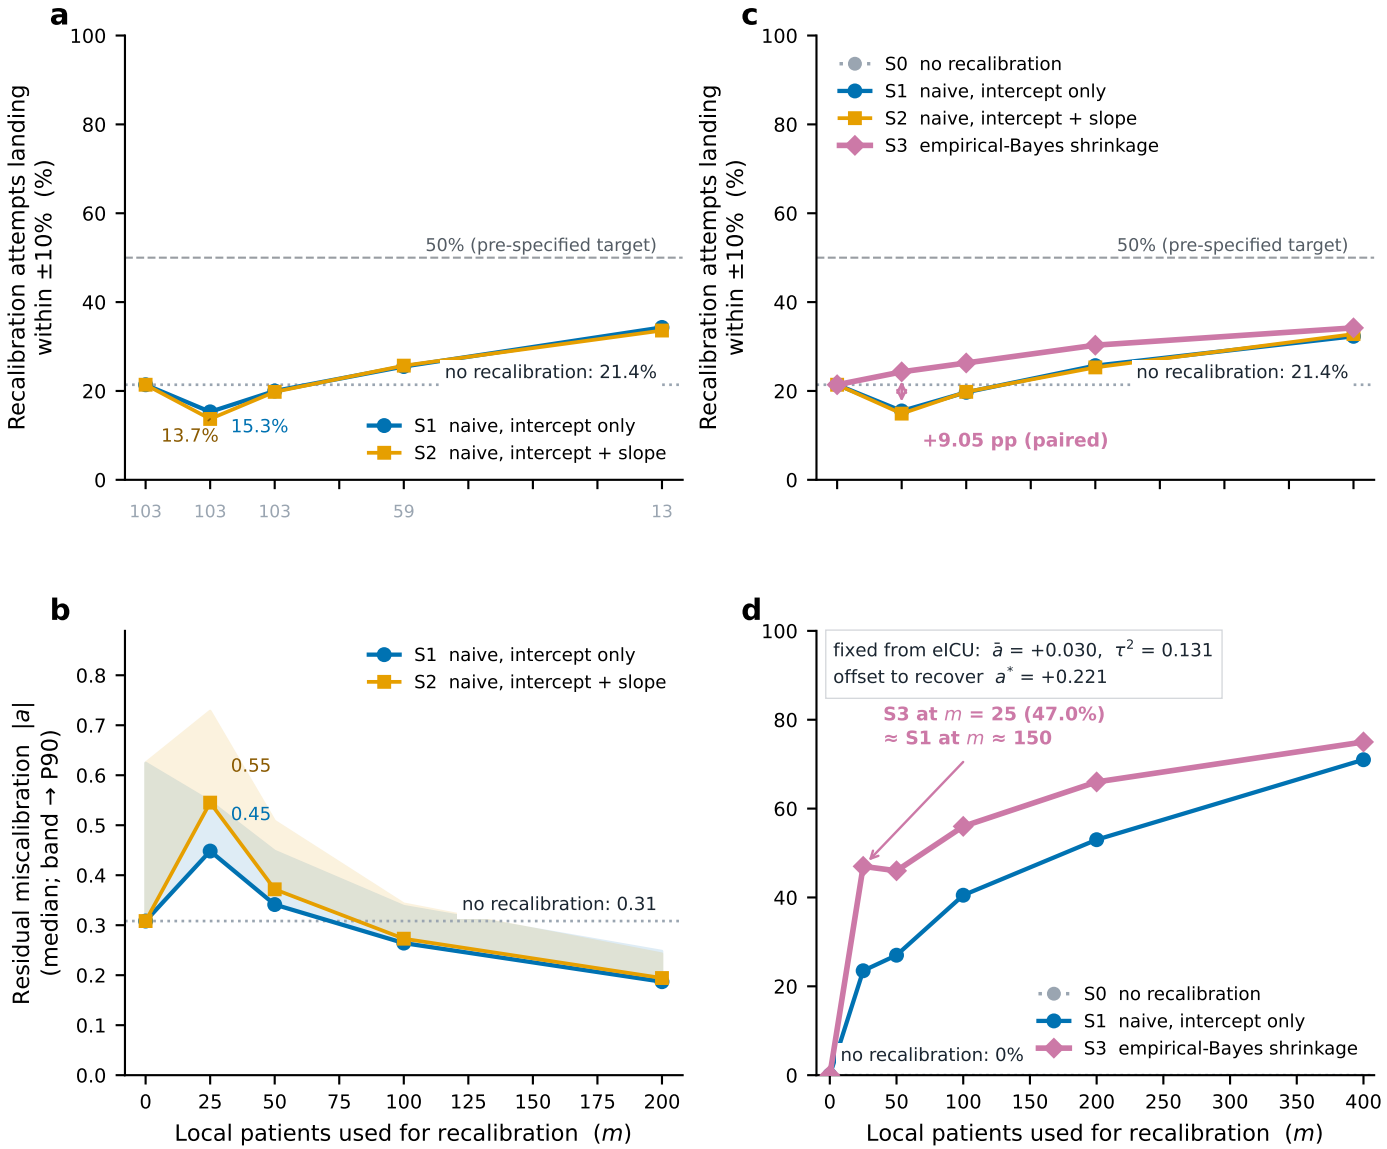
a
Recalibration attempts landing within ±10% (%)
50% (pre-specified target)
no recalibration: 21.4%
13.7%
15.3%
S1 naive, intercept only
S2 naive, intercept + slope
103
103
103
59
13
b
Residual miscalibration |a| (median; band → P90)
S1 naive, intercept only
S2 naive, intercept + slope
0.55
0.45
no recalibration: 0.31
Local patients used for recalibration (m)
c
S0 no recalibration
S1 naive, intercept only
S2 naive, intercept + slope
S3 empirical-Bayes shrinkage
50% (pre-specified target)
no recalibration: 21.4%
+9.05 pp (paired)
d
fixed from eICU: ā = +0.030, τ² = 0.131
offset to recover a* = +0.221
S3 at m = 25 (47.0%)
≈ S1 at m ≈ 150
no recalibration: 0%
S0 no recalibration
S1 naive, intercept only
S3 empirical-Bayes shrinkage
Local patients used for recalibration (m)