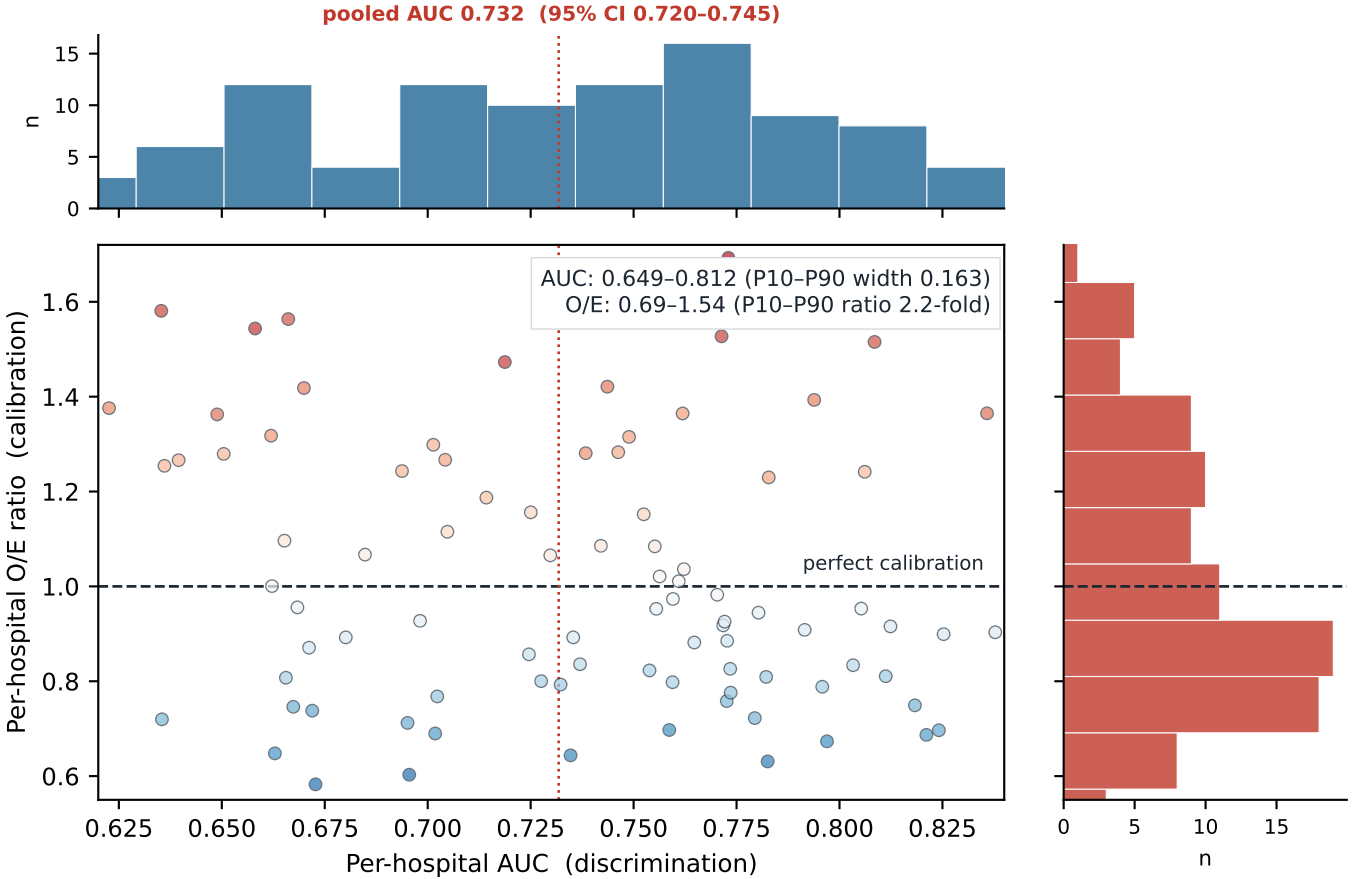
pooled AUC 0.732 (95% CI 0.720–0.745)
n
AUC: 0.649–0.812 (P10–P90 width 0.163)
O/E: 0.69–1.54 (P10–P90 ratio 2.2-fold)
perfect calibration
Per-hospital O/E ratio (calibration)
Per-hospital AUC (discrimination)
n