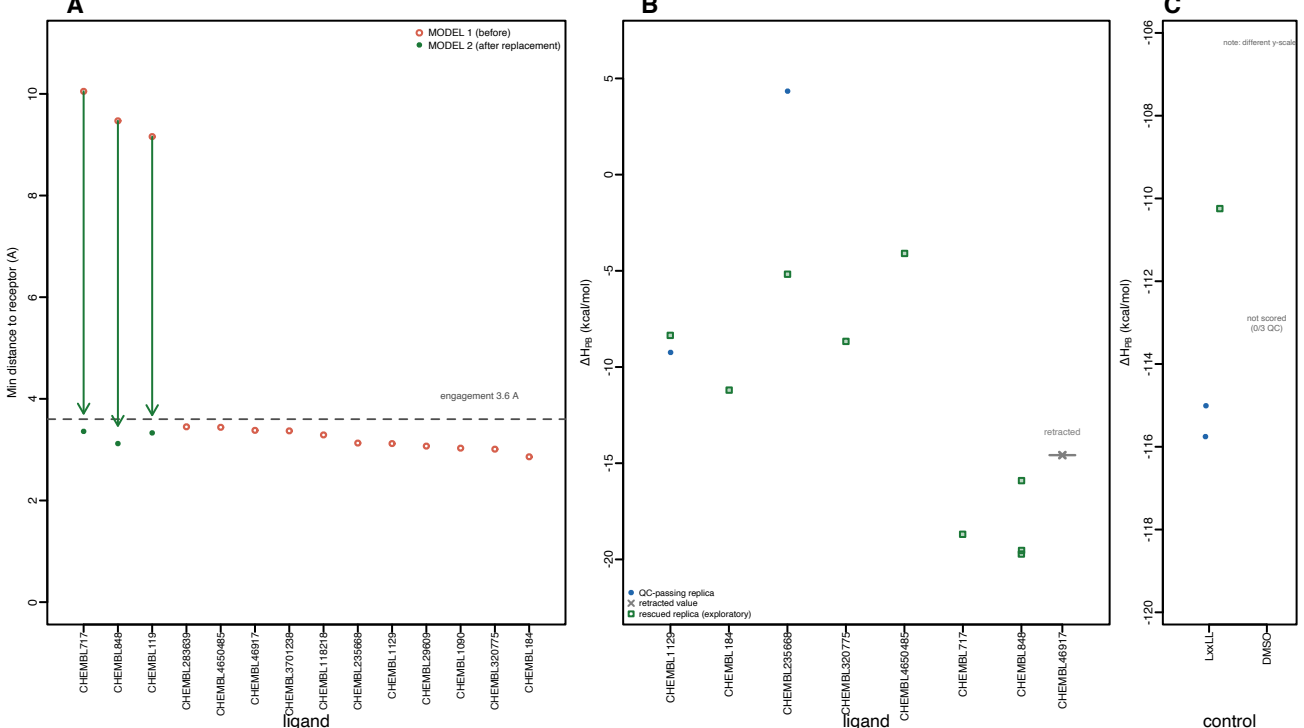
A
MODEL 1 (before)
MODEL 2 (after replacement)
Min distance to receptor (A)
engagement 3.6 A
CHEMBL717
CHEMBL849
CHEMBL119
CHEMBL283639
CHEMBL4650485
CHEMBL46917
CHEMBL3701239
CHEMBL118219
CHEMBL235669
CHEMBL1129
CHEMBL29609
CHEMBL1090
CHEMBL320775
CHEMBL184
ligand
B
ΔH_PB (kcal/mol)
retracted
QC-passing replica
retracted value
rescued replica (exploratory)
CHEMBL1129
CHEMBL184
CHEMBL235669
CHEMBL320775
CHEMBL4650485
CHEMBL717
CHEMBL849
CHEMBL46917
ligand
C
note: different y-scale
not scored
(0/3 QC)
ΔH_PB (kcal/mol)
LxxLL
DMSO
control