



## **In-House Fabrication of 1.3 to 7 mm MAS Drive Caps using Desktop 3D Printers**

Cyriaque Amerein, Utsab Banerjee, Zhenfeng Pang, Wenqing Lu, Vanessa Pimenta, Kong Ooi Tan

### **► To cite this version:**

Cyriaque Amerein, Utsab Banerjee, Zhenfeng Pang, Wenqing Lu, Vanessa Pimenta, et al.. In-House Fabrication of 1.3 to 7 mm MAS Drive Caps using Desktop 3D Printers. *Journal of Magnetic Resonance*, In press, pp.107391. 10.1016/j.jmr.2023.107391 . hal-03984013

**HAL Id: hal-03984013**

**<https://hal.science/hal-03984013>**

Submitted on 11 Feb 2023

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# **In-House Fabrication of 1.3 to 7 mm MAS Drive Caps using Desktop 3D Printers**

Cyriaque Amerein<sup>a,#</sup>, Utsab Banerjee<sup>a,#</sup>, Zhenfeng Pang<sup>a</sup>, Wenqing Lu<sup>b</sup>, Vanessa Pimenta<sup>b</sup>, and Kong Ooi Tan<sup>a,\*</sup>

<sup>a</sup>Laboratoire des Biomolécules, LBM, Département de Chimie, École Normale Supérieure, PSL University, Sorbonne Université, CNRS, 75005 Paris, France

<sup>b</sup>Institut des Matériaux Poreux de Paris, Ecole Normale Supérieure, ESPCI Paris, CNRS, PSL University, 75005 Paris, France

# denotes equal contributions

\*Corresponding Author:

Kong Ooi Tan

Laboratoire des Biomolécules, LBM, Département de Chimie,  
École Normale Supérieure, PSL University, Sorbonne Université, CNRS,  
75005 Paris, France

ORCID:0000-0002-3094-3398

E-Mail: [kong-ooi.tan@ens.psl.eu](mailto:kong-ooi.tan@ens.psl.eu)

Keywords: Magic-Angle Spinning, Solid-State NMR, 3D Printing, Additive Manufacturing

## **Abstract**


The 3D-printing technology has emerged as a well-developed method to produce parts with considerably low cost and yet with high precision ( $< 100\ \mu\text{m}$ ). Recent literature has shown that the 3D-printing technology can be exploited to fabricate a magic-angle spinning (MAS) system in solid-state nuclear magnetic resonance (NMR) spectroscopy. In particular, it was demonstrated that advanced industry-grade 3D printers could fabricate 3.2 mm MAS drive caps with intricate features, and the caps were shown to spin  $> 20\ \text{kHz}$ . Here, we show that not only lab-affordable benchtop 3D printers can produce 3.2 mm drive caps with a similar quality as the commercialized version, but also smaller 2.5 mm and 1.3 mm MAS drive caps—despite a slight compromise in performance. All in-house fabricated drive caps (1.3 to 7 mm) can be consistently reproduced ( $> 90\ \%$ ) and achieve excellent spinning performances. In summary, the  $> 3.2\ \text{mm}$  systems have similar performances as the commercial systems, while the 2.5- and 1.3-mm caps can spin up to  $26\ \text{kHz} \pm 2\ \text{Hz}$ , and  $46\ \text{kHz} \pm 1\ \text{Hz}$ , respectively. The low-cost and fast in-house fabrication of MAS drive caps allows easy prototyping of new MAS drive cap models and, possibly, new NMR applications. For instance, we have fabricated a 4 mm drive cap with a center hole that could allow better light penetration or sample insertion during MAS. Besides, an added groove design on the drive cap allows an airtight seal suitable for probing air- or moisture-sensitive materials. Moreover, the 3D-printed cap was shown to be robust for low-temperature MAS experiments at  $\sim 100\ \text{K}$ , making it suitable for DNP experiments.

## 1. Introduction

Solid-state NMR is a powerful characterization technique that has been widely applied to study solid-state samples ranging from small molecules, biological macromolecules, to inorganic materials.<sup>1</sup> Although solid-state samples usually have broad peaks due to anisotropic interactions such as dipolar couplings and chemical-shift anisotropy, they can be averaged out by performing magic-angle spinning (MAS) experiments,<sup>2,3</sup> where the sample is spun at an angle of  $54.74^\circ$  with respect to the static magnetic field. It is essential that the MAS frequency ( $\nu_r$ ) should be sufficiently larger than the size of the anisotropic interactions to achieve an efficient line-narrowing effect, i.e., the rotors can spin up to  $\nu_r=160$  kHz depending on their size (**Table 1**).<sup>4,5</sup> To achieve such fast MAS frequencies without significantly heating the NMR sample, the rotors are pneumatically spun with gas to reduce frictional heating. Besides achieving faster MAS frequencies, maintaining a stable spinning frequency (usually within a deviation of few Hz) is important over the course of experiments, especially for 2D or 3D NMR experiments that could last several days or week(s). Hence, the choices of material for both the rotor and MAS drive cap are important as they must be mechanically rigid (high tensile or flexural strength), and easily fabricated—especially the drive cap with an intricate spiral feature. Some of the materials that fulfill these criteria are  $\text{ZrO}_2$ , Macor®, boron nitride, Kel-F®, Vespel®, and Torlon®. Among these choices,  $\text{ZrO}_2$  and Vespel are popular materials for the drive cap because  $\text{ZrO}_2$  has superior mechanical strength and a low thermal expansion coefficient, which is preferred for low-temperature dynamic nuclear polarization (DNP) experiments.<sup>6–8</sup> However, machining  $\text{ZrO}_2$  is challenging and, hence, expensive, i.e. a 3.2mm  $\text{ZrO}_2$  cap costs ~1k USD (CortecNet). Although the Vespel drive cap is more affordable (~130 USD for 3.2 mm), it is still a non-negligible expense because the delicate fins on the drive cap wear out easily if they are mishandled or after repeatedly fitted/removed from the rotor. These effects are noticeably noted for smaller rotors, i.e., the 0.7 mm drive cap is usually for one-time use only, and it has to be replaced with a new piece when packing new samples into the same rotor. To minimize the expenditure on these consumables (MAS drive caps), it has been recently demonstrated that the MAS drive caps can be fabricated using relatively low-cost 3D printing technology.<sup>9,10</sup>

There are two main categories of 3D printing technology: fused deposition modelling (FDM) and stereolithography (SLA). Although the FDM method has, in general, a poorer resolution, it is more affordable and easier to use relative to the resin-based SLA method. Both

3D printing technologies have been exploited in various NMR applications, ranging from fabricating MAS sample eject systems,<sup>11</sup> RF coils,<sup>12–15</sup> NMR sample tubes,<sup>16</sup> parahydrogen generator,<sup>17</sup> NMR sample degassing apparatus,<sup>18,19</sup> NMR probeheads,<sup>20</sup> etc. Besides these examples, Xu et al. have recently demonstrated that it is possible to fabricate MAS stator and drive caps using FDM, but only for > 3.5 mm system.<sup>9</sup> High-resolution SLA technology has also been exploited for constructing MAS spinning system. Notable examples include the fabrication of > 4 mm spherical-rotor stators using a benchtop 3D printer by the Barnes' group,<sup>21,22</sup> and a 3.2 mm cylindrical-rotor stator and drive caps produced by dedicated manufacturing companies reported by Banks et al.<sup>10</sup> Although outsourcing the manufacturing process can save labour resources, we note that the quality of the parts varies across different batches. This could be because the printing and/or post-processing steps performed by the company are not necessarily the same for each batch. Consequently, the lack of consistent results could lead to a more time- and cost-consuming process. Moreover, the same publication commented that the benchtop 3D printer (Form3 with 25  $\mu\text{m}$  XY resolution) was tested to be incapable of producing the 3.2 mm drive caps.<sup>10</sup> In this publication, we re-examine this statement by showing that not only the Form3+ 3D printer can fabricate robust 3.2 mm drive caps, but also smaller 2.5- and 1.3-mm drive caps (with slightly compromised performances). In particular, the 3.2 mm 3D-printed drive caps (**Fig. 1**) can spin up to  $\nu_r = 22 \text{ kHz} \pm 1.3 \text{ Hz}$  (**Table 1**), which has similar performances as the commercial versions, but only costs < 1 US cents and 5 minute/piece to be 3D-printed (assuming a simultaneous printing of 100 pieces in a single print job). Additionally, the in-house fabricated 3D-printed drive caps exhibit excellent spinning stability that is sufficient for practical multi-dimensional MAS NMR experiments.

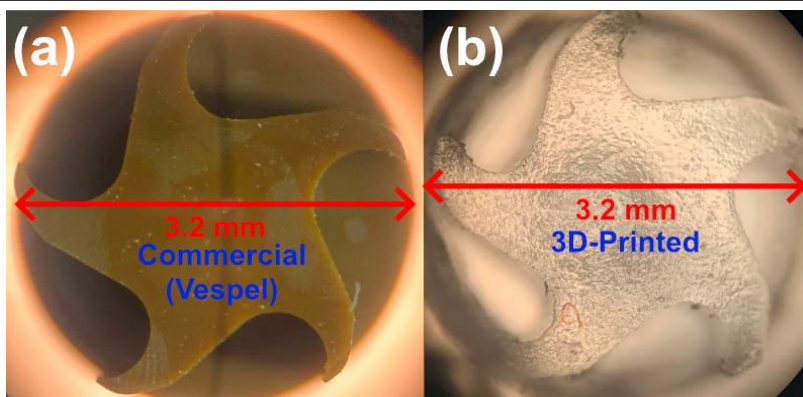


**Figure 1:** Image of (a) a commercial (Bruker) Vespel and (b) a 3D-printed 3.2 mm MAS drive cap.

## 2. Experimental Methods

### 2.1. 3D Printing and Post-Processing Methods

The drive caps were designed in Autodesk Inventor (Autodesk Inc, San Rafael) following a similar design described in Banks et al.<sup>10</sup> The drive caps were printed using standard Clear v4 resin in a Form 3+ (Formlabs) printer with a 25  $\mu\text{m}$  XY resolution and layer thickness. The 3D printer costs ~4 k USD, and the resin costs ~140 USD/litre. The printing supports were placed on the bottom of the stem with a contact point size of 0.3 mm. It takes ~4 hours to simultaneously 3D-print 100 pieces of drive caps in a single print job. Note that the build platform of the 3D printer can accommodate more than 100 pieces in a single print (if needed) without significantly increasing the printing hours. After the printing job finished, the parts were first rinsed in an isopropanol-water mixture (9:1 by volume ratio) to remove the uncured resin and irregularities on the surface. Then, the supports were removed and rinsed again before being cured under UV light (Elegoo Mercury) for 1 h (2x30 min, with another rinsing step between the two curing sessions) to enhance the mechanical properties. Note that the caps should be completely dry after every rinsing step. It is known that the SLA-printed parts gradually shrink in size over time, and the long curing time (1 hr) is a crucial step to accelerate the shrinking process and, hence, more stable in the long term.

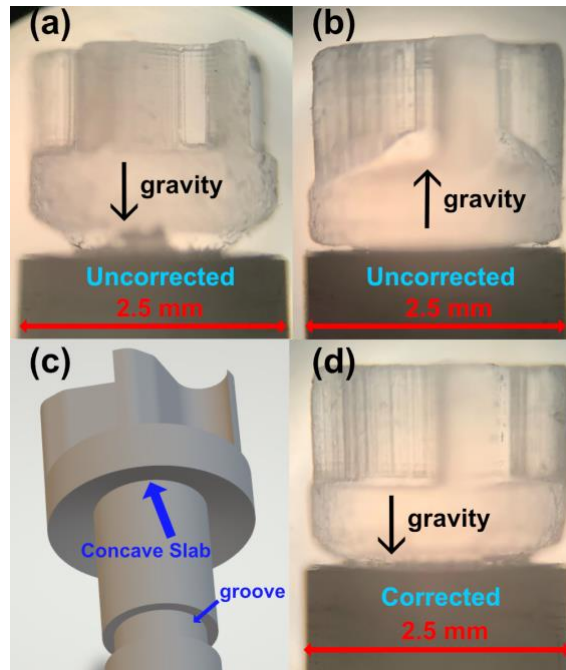


**Figure 2:** Images of 2.5 mm MAS drive caps. Note the undesirable overhang effect present in the (a) upright and (b) reversed orientation. The artefacts were compensated by designing (c) a concaved (curved inward) slab, which yields the (d) corrected cap that improves the maximum spinning frequency from 22 to 26 kHz.

To account for the change in dimension after the post-processing steps, we have iteratively compensated for the changes by redesigning and reprinting the parts. In addition to the Form 3+ 3D printer, we have also tested another benchtop 3D printer (Elegoo Saturn), which has a lower XY resolution (50  $\mu\text{m}$ ). We have used the Elegoo 3D printer to print 4 mm caps (with Elegoo standard grey resin), and they show similar performances as the commercial (Bruker) version.

## 2.2. Artefact Compensation by Iterative Design Modification

Note that the dimensions of the 3D-printed pieces could be slightly different from the computer-aided design (CAD) due to the properties of the resins, printing environment (temperature), post-processing steps, printing orientations, etc. Nevertheless, some of these undesired changes could be compensated by minor modifications (often iterative) in the CAD. An example of this is the ‘overhang’ feature that occurs when the resin tends to bulge downward due to gravity (**Fig. 2a**). The artefact has resulted in a small gap between the drive cap and the rotor and, hence, compromised the spinning performances, i.e., it does not spin up beyond 22 kHz. Although this feature can be partially compensated by reversing the printing orientation, it, unfortunately, affects the form of the fins (**Fig. 2b**). Thus, we introduced a concave curvature to the horizontal slab (**Fig. 2c**). Consequently, the printed part (**Fig. 2d**) did result in a better fit and a higher spinning frequency to ~26 kHz. Besides that, we have also made the fins on the 1.3 mm drive cap sharper

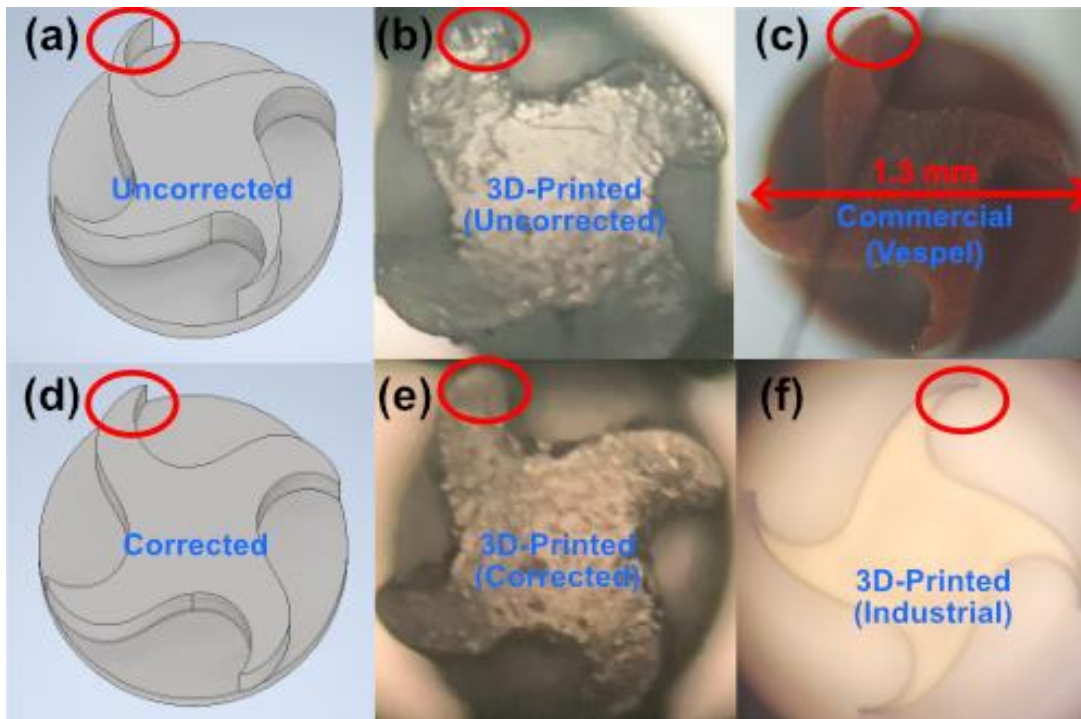

**Figure 3:** 1.3 mm MAS drive caps. Images of the (a and d) CAD and (b and e) 3D-printed pieces (a and b) before and (d and e) after the design compensation. Images of the (c) machined and (f) industrial 3D-printed (BMF) drive caps.

(**Fig. 3d** and **e**) to compensate for the broader-than-expected fins (**Fig. 3a** and **b**) due to the finite size of the laser beam used in the Form 3+ 3D printer (85  $\mu\text{m}$ ). The corrected drive caps (**Fig. 3e**) were able to achieve the same spinning frequency with less drive gas (vide infra, **Fig. 6a**), and the maximum  $\nu_r$  was improved from 37 to 45 kHz. Additionally, we would like to highlight that the diameters of the stem (the component that fits into the rotor) and the slab (**Fig. 2c**) of the drive caps require very tight tolerances, i.e., they must be fabricated within a  $\sim 10\ \mu\text{m}$  accuracy for optimal performances. At last, we emphasize that such iterative compensation is possible only because the 3D printing protocol yields very consistent and reproducible results. We have fabricated many batches of the drive caps over several months, and they yield very similar results.

Diameter (mm)	Volume ( $\mu\text{l}$ )	Max $\nu_r$ of machined Vespel cap (kHz)	Max $\nu_r$ of 3D-printed cap (kHz)	Printing consistency
7	240	7	6 kHz $\pm$ 0.5 Hz	<100 %
4	70	15	10 kHz $\pm$ 1.6 Hz (Elegoo, no hole) 7 kHz $\pm$ 0.3 Hz (Elegoo, with hole)	<100 %
3.2	30	24 (RT) 12 ( $\sim$ 100 K)	22 kHz $\pm$ 1.3 Hz. (RT) 8 kHz $\pm$ 2 Hz ( $\sim$ 100 K)	<100 %
2.5	12	35	26 kHz $\pm$ 2.1 Hz	95 %
1.3	2.5	67	46 kHz $\pm$ 1.1 Hz (Form3+) 60 kHz $\pm$ 3.4 Hz (BMF)	92 %


**Table 1:** Summary of rotor sizes, spinning frequencies, and other specifications of both commercial (Vespel) and 3D-printed MAS drive caps. We have tested at least 10 pieces for each rotor size, except for the industrial-printed (BMF) 1.3 mm drive cap, where only two out of three available pieces were tested. We have only examined the 3.2 mm cap at  $\sim 100\ \text{K}$  only once for  $\sim 17$  hours. RT refers to room temperature.

### 2.3. MAS Experiments using 3D-Printed Caps

The 3D-printed caps were fitted into standard  $\text{ZrO}_2$  rotors for MAS experiments in Bruker MAS probes or a benchtop spinning station at ambient temperature. A Bruker MAS II unit was used to regulate the drive and bearing gas pressure to achieve a stable spinning frequency. We have tested at least 10 pieces of each design for at least 15 minutes to evaluate the MAS performance. The pressure of each gas inlet and spinning frequency as a function of time in the automated



mode were logged using TopSpin (Bruker). We have tested the 3.2 mm drive caps on both  $\text{ZrO}_2$  and sapphire rotors. All zirconia rotors fitted with 3D-printed caps spun  $> 20$  kHz without major issues. However, the sapphire rotor crashed when spun above 18 kHz (rated for 15 kHz at RT). For the 1.3 mm drive caps printed with an industrial 3D printer (Boston Micro Fabrication (BMF)), we have tested only 2 out of the 3 ordered pieces.

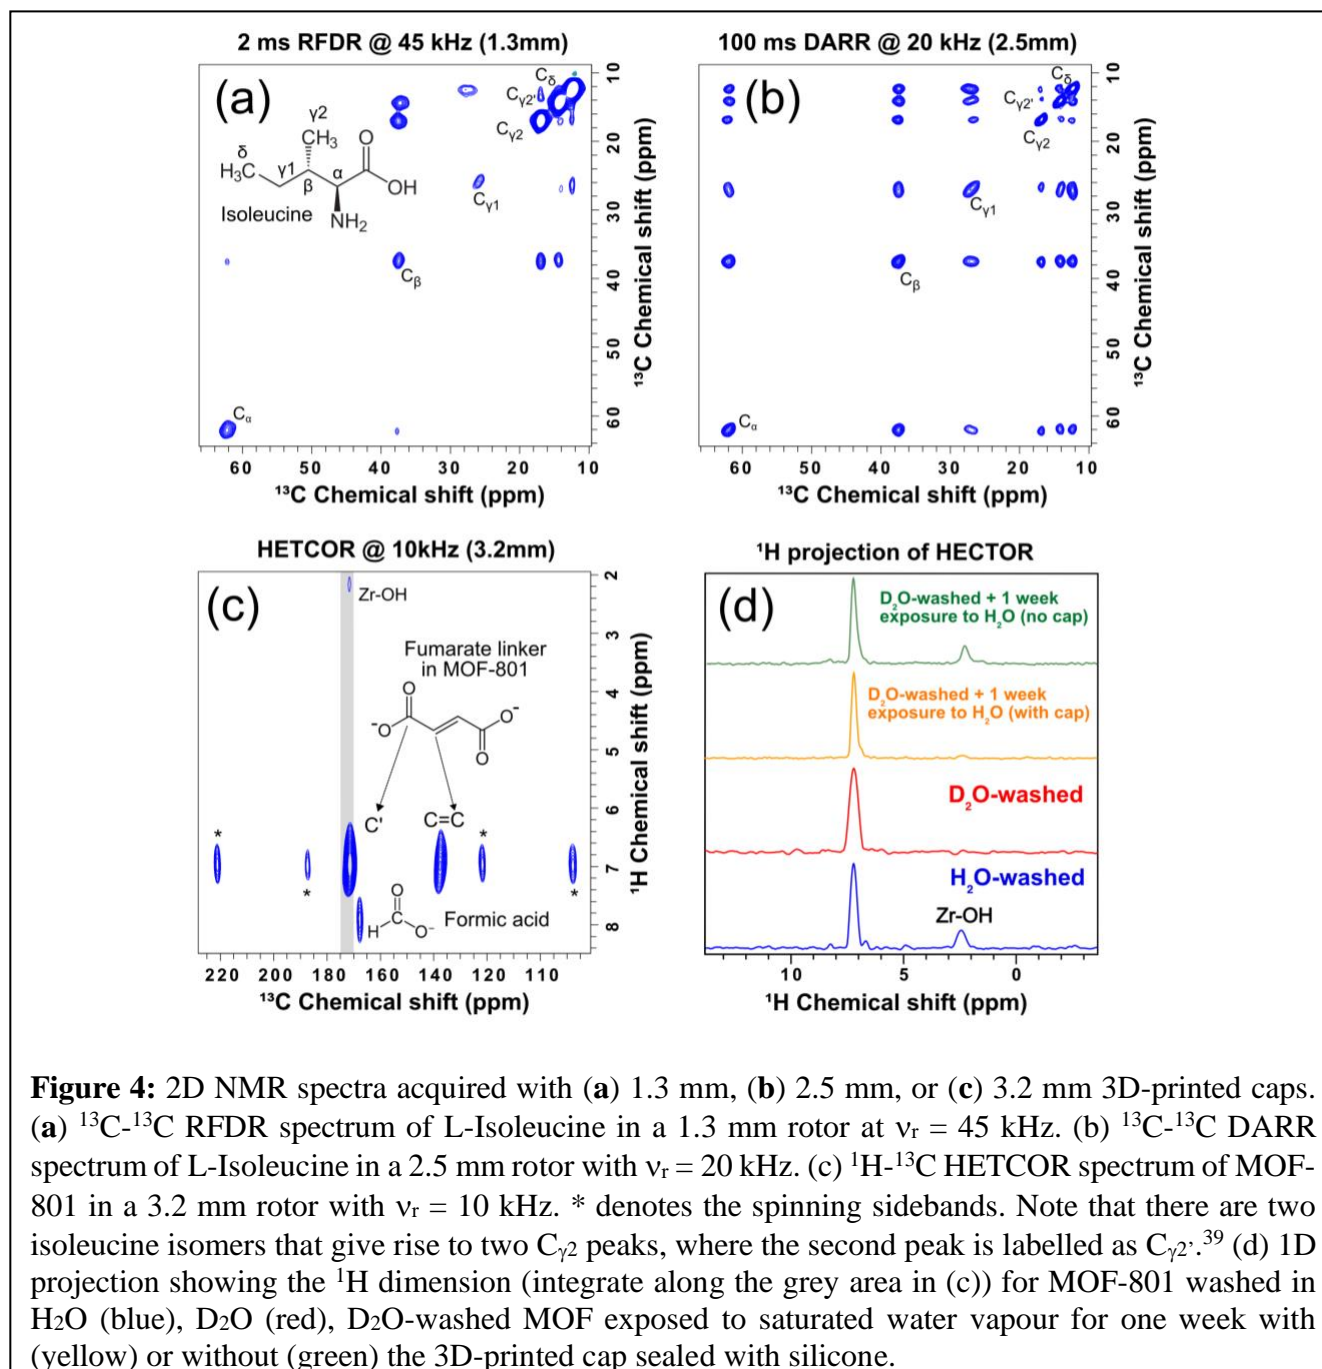

## 2.4. NMR Samples and Experiments

The  $^{13}\text{C}$ - $^{15}\text{N}$  L-Isoleucine sample was purchased from CortecNet and used without further purification. For the Metal-Organic Framework (MOF-801) sample,<sup>23</sup> the MOF was synthesized through an established procedure and washed with  $\text{D}_2\text{O}$  using ultrasounds.<sup>23</sup> The  $\text{D}_2\text{O}$  washing step was performed to promote an exchange of the hydroxyl proton ( $\text{Zr-OH}$ ) with deuterium, which helps unambiguously assign the  $\text{Zr-O}^1\text{H}$  NMR peak observed in an  $\text{H}_2\text{O}$ -washed MOF sample. The  $\text{D}_2\text{O}$ -washed MOF sample was then activated in a vacuum drying oven for 12 hours at  $100^\circ\text{C}$  to remove excess solvent. To minimize the exposure of the dried MOF sample to the moist in the atmosphere, the sample was packed into a 3.2 mm rotor closed with a 3D-printed drive cap sealed with silicone-filled (Bluestar CAF 1) groove inside an argon-filled glove box.

The NMR spectra were acquired using an 800 MHz spectrometer equipped with an Avance Neo console (Bruker). We have used either a 1.3 mm, 2.5 mm, or 3.2 mm (E-free) triple-channel MAS probe to perform MAS NMR experiments. The  $^1\text{H}$  and  $^{13}\text{C}$  chemical shifts were referenced to the adamantane signal at 38.5 ppm on the tetramethylsilane (TMS) scale. The RFDR experiment (**Fig. 4a**) was performed using the 1.3 mm probe at 45 kHz MAS frequency with a  $\sim 2$  ms RFDR mixing time. The DARR experiment (**Fig. 4b**) was performed using the 2.5 mm probe at  $\nu_r = 20$  kHz with a 100 ms DARR mixing time. The HETCOR spectra (**Fig. 4c & d**) were acquired using a 3.2 mm probe at  $\nu_r = 10$  kHz. The experimental time for each 2D experiment is  $\sim 2$  hr. The magic angle and field  $B_0$  homogeneity were optimized with KBr and adamantane, respectively. The low-temperature MAS experiment (Fig. 7) was performed using a 3.2 mm HXY MAS DNP probe (Bruker). The sapphire rotor was packed with MOF-801, the surface of which was wetted with solutions of DNP juice ( $d_8$ -glycerol:  $\text{D}_2\text{O}$ :  $\text{H}_2\text{O}$  in 6:3:1 by volume) doped with 5 mM TinyPol. We filled the groove on the 3D-printed drive cap with red silicone sealant so that the cap does not become loose as it shrinks at low temperatures.<sup>11</sup> Prior to the MAS experiment, the rotor was immersed in liquid nitrogen at  $\sim 77$  K to ensure that the 3D-printed cap remained intact and well-fitted to the rotor. We initially planned to perform DNP experiments with the 3.2 mm system, but the gyrotron was not operational during the experiment. Nevertheless, we performed conventional NMR experiments at low temperatures without microwaves, which allows the sample to reach a colder temperature ( $\sim 105$  K) due to the absence of microwave heating. The stator temperature was maintained at  $\sim 109$  K (measured at stator after the mixing of the variable temperature (VT), bearing, and drive gas) by regulating the temperature of the three spinning gases at the probe base to be  $\sim 95$  K. Hence, we estimated the actual sample temperature to be  $\sim 100$  K.


## Results and Discussions

A statistical summary of the MAS tests performed on the 1.3 to 7 mm drive caps is tabulated in **Table. 1**. The max  $\nu_r$  is defined as the maximum spinning frequency we have tested, and it is intentionally chosen to be slightly below the specification of the commercial (Bruker) caps to avoid rotor-crash incidents. We found that the in-house 3D-printed drive caps for sizes  $\geq 3.2$  mm have almost equivalent MAS performances as the commercial caps, while the cost of 3D printing is almost negligible. Nevertheless, the smaller 3D-printed drive caps (1.3 mm and 2.5 mm) yield less satisfactory spinning performances than the machined caps. Hence, we improvised the original CAD to compensate for the printing inaccuracies (vide supra), which moderately improved the maximum  $\nu_r$  to  $> 70$  % of those specified for the commercial caps, i.e., the 2.5- and 1.3-mm 3D-printed caps can spin up to 26 and 46 kHz, respectively. Despite the lower max  $\nu_r$ , the 3D-printed caps still achieve excellent spinning stability ( $\leq 2$  Hz), which is practical for MAS NMR experiments.

To further assess the transfer efficiency of the momentum from the gas to the printed drive, we have recorded the spinning profiles (**Fig. 6**) of the smaller caps as a function of the drive gas pressure. We noted that the 3D-printed 1.3 mm caps are less efficient and require more drive gas to reach the same spinning frequency as the commercial caps.<sup>24,25</sup> We hypothesized that the 1.3 mm caps could spin faster if they could be more accurately made. To test our hypothesis, we have 3D-printed the 1.3 mm caps using a state-of-the-art industrial 3D printer (BMF) with HTL resin, which has a  $\sim 12\times$  higher XY resolution (2  $\mu\text{m}$ ) than our desktop Form 3+ printer. Not only the BMF cap exhibits sharper fins (circled in **Fig. 3f**) than those made by Form 3+ (**Fig. 3e**), but also those machined Vespel caps (**Fig. 3c**). Indeed, those industrial-printed caps were able to achieve  $\nu_r = 60 \text{ kHz} \pm 3 \text{ Hz}$  (**Fig. 5b**). Note that we have only tested two out of three available pieces. Both pieces achieve similar spinning frequencies with the same bearing and drive gas, but the second piece broke when spun above 50 kHz. This issue could be mitigated if harder materials (alumina ceramics or *HT 200* from BMF) are used for printing the caps, but they are not in-house fabricated and are beyond the scope of this work. Although these industrial 3D-printed caps cost  $> 20$  USD / piece (for a large-quantity order), they are still an order of magnitude cheaper than the machined Vespel caps.

On the printing consistency, which we defined as the ratio of the number of pieces that spin to the total number of printed parts, we have achieved very consistent results, i.e., all printed drive caps can be reliably reproduced with  $> 90$  % consistency. Note that it is necessary to spin-test


the printed drive caps  $\leq 2.5$  mm, as the defective drive caps cannot be easily identified with visible features. For  $\geq 3.2$  mm drive caps, they are remarkably near 100 %. For the most used 3.2 mm system, we have repeatedly fabricated more than 100 pieces over few months using the same optimized protocol, and they have all worked. We have also tested both freshly printed and several-month-old pieces, and they yield equal performances. It is noteworthy to be aware that

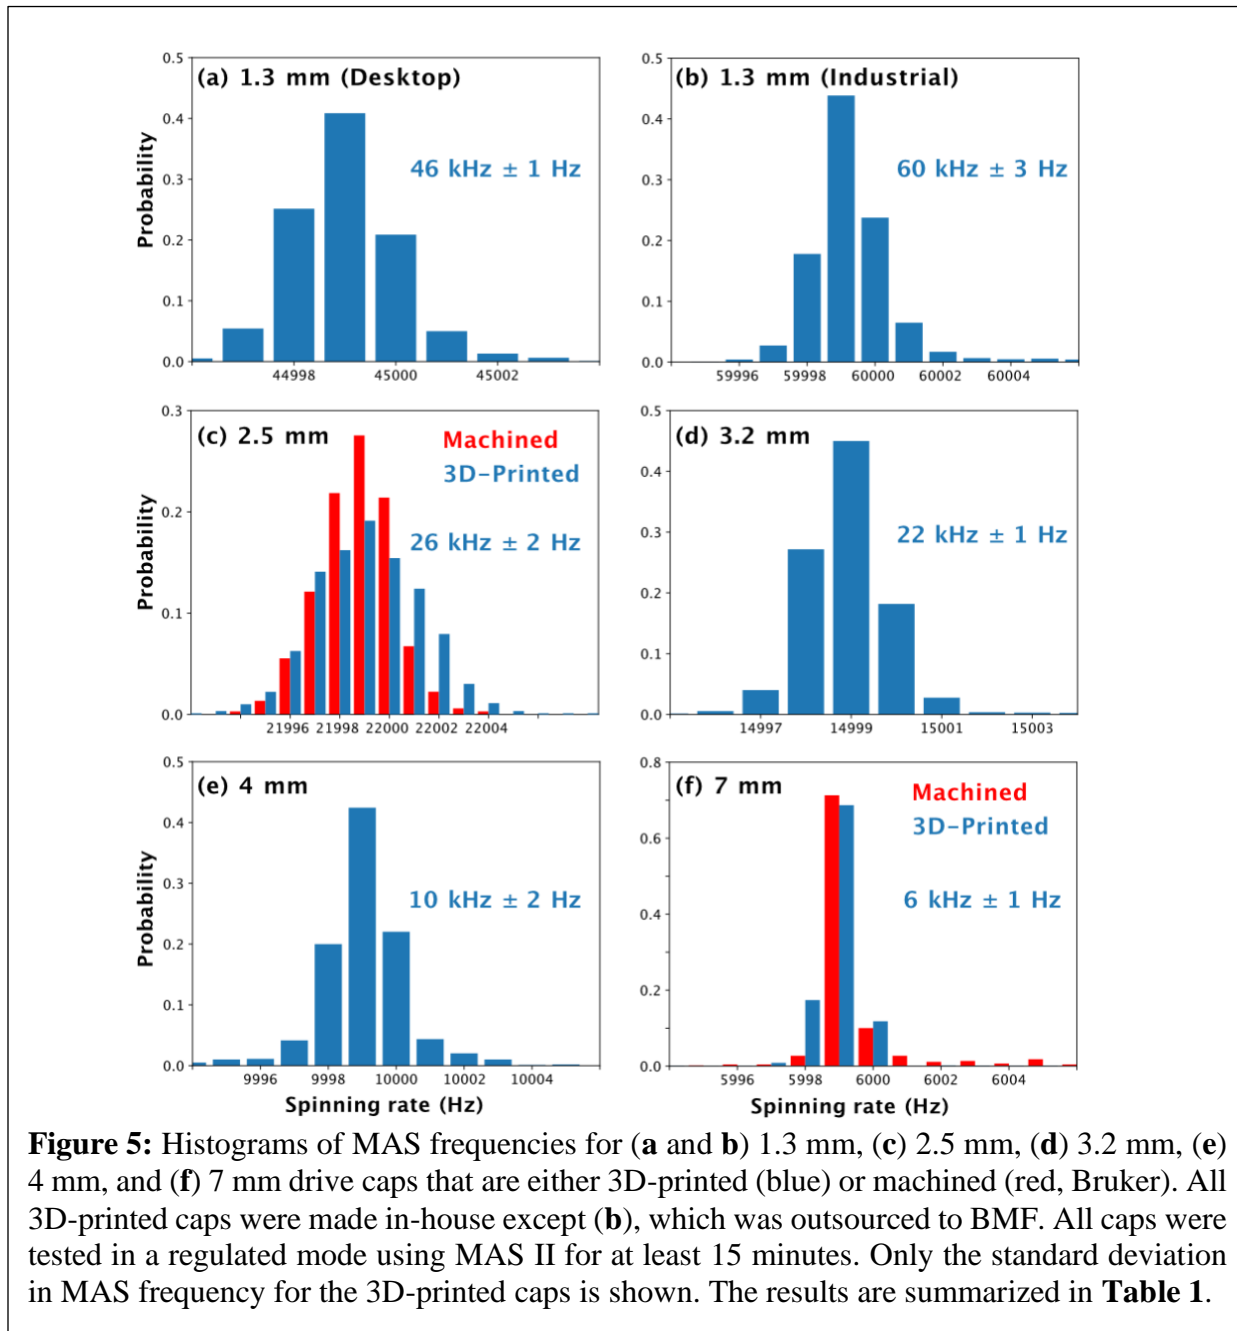

we did not reuse any old caps because the cost is almost negligible.

To assess if the 3D-printed drive caps are practical for long MAS NMR experiments, we have performed various 2D NMR correlation experiments on the 1.3 mm, 2.5 mm, and 3.2 mm drive caps on standard compounds. Among these experiments, the RFDR dipolar recoupling


experiment performed on the 1.3 mm rotor requires the rf pulses to be rotor-synchronized to yield an efficient correlation between the  $^{13}\text{C}$  peaks.<sup>26</sup> The fact that the 2D spectra show excellent linewidths and all the expected cross peaks, we conclude that the homebuilt 3D-printed drive caps

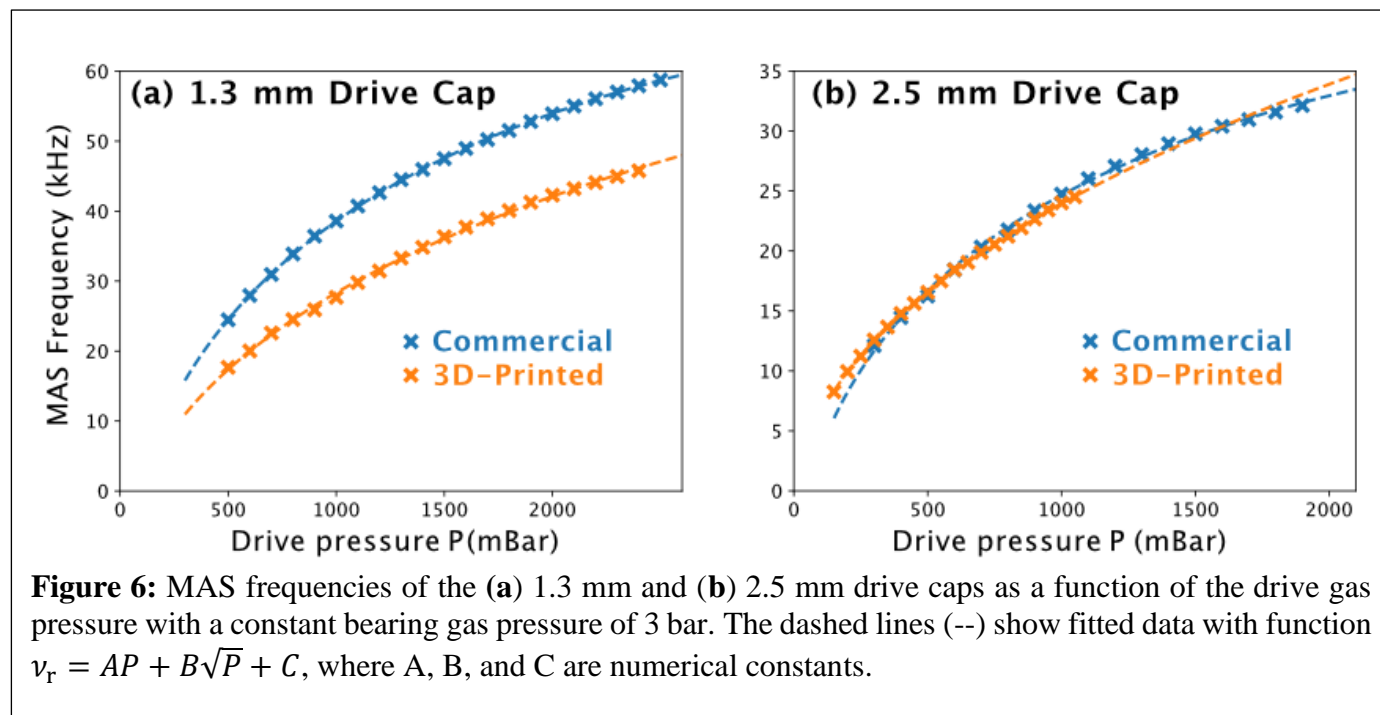

are practical for actual MAS NMR experiments.

In addition to the standard drive cap designs, we also prototyped new models that could be useful for special NMR applications. For instance, we have added a groove to the stem (**Fig. 2c**) so that the rotor could be sealed using epoxy or silicone sealant, which is useful for studying air- or moisture-sensitive NMR samples. As proof of principle, we have applied such a protocol on a MOF-801 sample packed in a 3.2 mm rotor (see **Section 2.4**). MOF-801 is built-up from  $\text{Zr}_6\text{O}_4(\text{OH})_4$  oxo-clusters and fumaric acid molecules. The labile proton in the -OH groups could, in principle, exchange with deuterium. To test the hypothesis, we recorded some 2D  $^1\text{H}$ - $^{13}\text{C}$  HETCOR spectra (**Fig. 4c & d**) of MOF-801 prepared under various conditions. The  $^1\text{H}$  peak intensity at ~2.4 ppm is significantly lower than in the  $\text{D}_2\text{O}$ -washed sample relative to the  $\text{H}_2\text{O}$ -washed counterpart. This implies that labile  $^1\text{H}$  in Zr-OH could be exchanged with  $\text{D}_2\text{O}$  to form Zr-OD, which attenuates the  $^1\text{H}$  peak intensity. The experimental results allow us to unambiguously assign the observed  $^1\text{H}$  peak to Zr-OH, which was previously stated in literature with only DFT calculations.<sup>27</sup> To examine if the sealed 3D-printed cap is sufficiently robust for studying moisture-sensitive samples, we put the rotors packed with  $\text{D}_2\text{O}$ -washed samples inside Eppendorf vials filled with a few drops of  $\text{H}_2\text{O}$  for ~1 week. For the rotor fitted with a silicone-sealed 3D-printed cap, the HETCOR spectrum (**Fig. 4d**) is nearly identical to the spectrum acquired before exposure to water vapor. In contrast, the rotor without a cap showed significant growth in the Zr-O $^1\text{H}$  peak.


Hence, the results confirm that the 3D-printed cap with silicone seals provides a robust airtight condition suitable for studying air- or moisture-sensitive NMR samples. Moreover, emptying the rotors fitted with silicone- or epoxy-sealed drive caps—which could become unusable if destructively removed—is more cost-efficient if the caps were 3D-printed in-house.

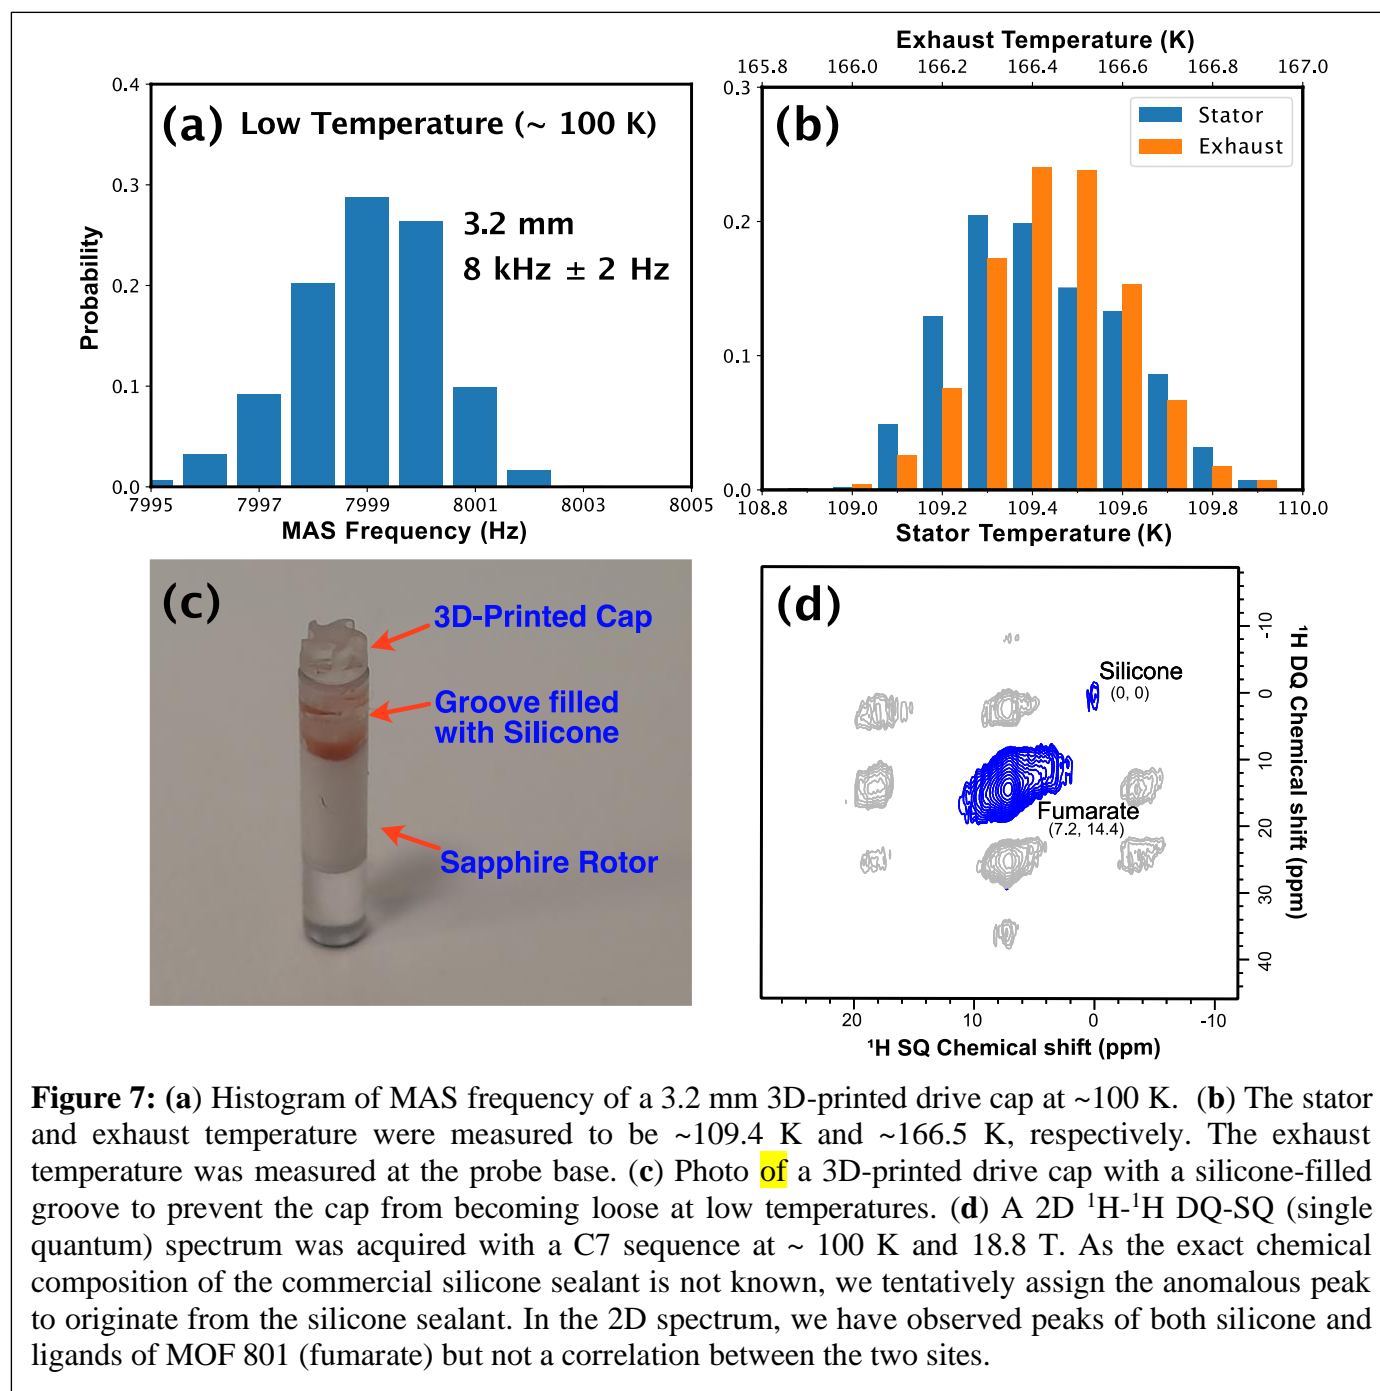

Another main concern about the 3D-printed drive caps is their feasibility for low-temperature applications. It was reported by Banks et al. that the 3D-printed caps fabricated by an industrial 3D printer (Protolabs) crack at ~ 100 K.<sup>10</sup> To examine our printed drive caps printed (Formlabs), we fitted a 3D-printed cap into a sapphire rotor packed with MOF-801 wetted with DNP juice (see

Experimental Section) and sealed with silicone sealant (**Fig. 7c**), before spinning it at  $\sim 100$  K using a 3.2 mm 800 MHz MAS DNP probe. Figure 7a shows the histogram of regulated MAS frequency of  $\nu_r = 8 \text{ kHz} \pm 2 \text{ Hz}$  at a sample temperature of  $\sim 100$  K over  $\sim 17$  hours. The recorded spinning frequency at low temperatures is slightly less stable than the room-temperature operation (**Fig. 5d**), possibly due to a larger standard deviation in stator temperature (see **Fig. 7b** and Experimental Section). Following that, we recorded a 2D  $^1\text{H}$ - $^1\text{H}$  double-quantum filtered (DQF) spectrum (**Fig. 7d**) using a symmetry-based C7<sub>2</sub><sup>1</sup> sequence, which is a rotor-synchronized dipolar recoupling sequence that requires a stable spinning frequency for efficient performance.<sup>28</sup> Hence, the 2D experiment acquired at  $\sim 100$  K demonstrates that the 3D-printed drive cap is robust for low-temperature (including MAS DNP) applications.

Besides that, we have also modelled 4 mm drive caps with a center hole (**Fig. 8**), which could be useful for in-situ monitoring of chemical reactions during MAS experiments, or those NMR experiments that require in-situ illumination of light or lasers.<sup>29–32</sup> For the first case, similar instrumentation and experiments were demonstrated in the literature,<sup>33–36</sup> where a reactant gas was directed into a 7 mm rotor via an injection tube through the drive cap with an axial hole. The 4 mm drive cap (without an injection tube) could spin till  $\nu_r = 7 \text{ kHz} \pm 0.3 \text{ Hz}$ , which is slightly slower than the normal cap ( $\sim 10 \text{ kHz}$ ).

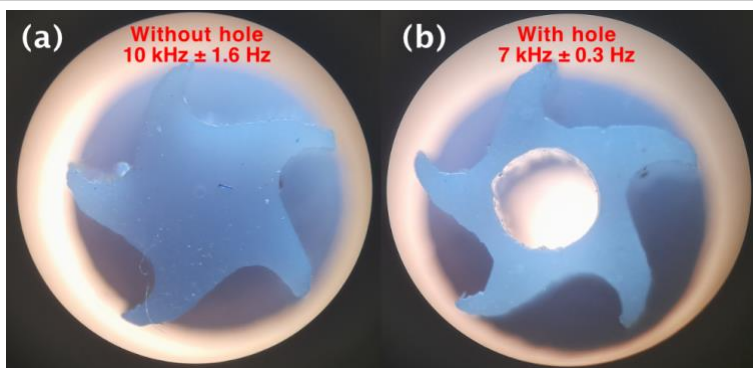

**Figure 8:** Image of the 4 mm drive cap (a) without or (b) with a center hole. The drive caps were printed using a desktop 3D printer (Elegoo Saturn). Their MAS performances are specified in the image.

### 3. Conclusion

We have demonstrated that it is possible to fabricate 1.3–7 mm drive caps using an affordable desktop 3D printer in-house. The moderate-accuracy but high-precision 3D printing method allows us to fabricate highly consistent ( $> 90\%$ ) MAS drive caps with similar results as the commercial caps for the  $\geq 3.2$  mm system. The smaller ( $\leq 2.5$  mm) caps can spin up to  $\sim 70\%$  as fast as the commercial caps, and yet with a high spinning stability ( $< 2 \text{ Hz}$ ). The high spinning stability of the

drive caps allows practical multidimensional NMR experiments to be performed. Additionally, we have exploited the high-resolution (2  $\mu\text{m}$ ) industrial 3D printer (BMF) to fabricate the 1.3 mm caps, which yield near equivalent MAS performances as the commercial caps. We foresee that it could be possible to 3D print smaller ( $\leq 0.7$  mm)<sup>4,5,37,38</sup> caps with similar or harder materials offered by the same company. In contrast to traditional machining, which becomes more challenging and expensive to fabricate smaller drive caps, 3D printing becomes cheaper as the size of the drive cap decreases—because more pieces could be simultaneously printed in a single print job on the platform. The relatively low cost and short fabrication time have allowed us to prototype new designs for new or custom MAS NMR applications. For instance, it costs less than 1 USD and 6 hours to fabricate 100 pieces of the MAS drive caps in-house. Not only does the silicone-filled groove on the 3D-printed cap provides an airtight environment suitable for studying air- or moisture-sensitive materials, but also allows low-temperature MAS experiment (including DNP) at  $\sim 100$  K. As the 3D printing technology continues to flourish, we expect higher-resolution 3D printers will become more easily accessible by laboratories, and new tools could be fabricated in-house for novel NMR experiments.

## Acknowledgements

We acknowledge Dr. Nicolas Birlirakis, Dr. Dan Banks, and Natalie Golota for helpful discussions. This work was supported by fundings obtained from the French National Research Agency: *PulsedDNP* (ANR-20-ERC9-0008) and *HFPulsedDNP* (ANR-21-CE29-0019), as well as RESPORE (n° 339299). Wenqing Lu acknowledges the China Scholarship Council for providing the funding (n° 201906880002).

**Supporting Information Available:** The designs of the drive caps (1.3, 2.5, 3.2, 4, and 7 mm) are available in the '.stl' and '.ipt' (Autodesk Inventor) format. In addition to 3D printing, we have machined a simple cap-removal tool to remove the drive caps from the rotors. A movie that shows the spinning of 3D-printed cap is available.



## **References**

- <sup>1</sup> B. Reif, S.E. Ashbrook, L. Emsley, and M. Hong, Nat. Rev. Methods Prim. **1**, 2 (2021).
- <sup>2</sup> E.R. Andrew, A. Bradbury, and R.G. Eades, Nature **182**, 1659 (1958).
- <sup>3</sup> I.J. Lowe, Phys. Rev. Lett. **2**, 285 (1959).
- <sup>4</sup> M. Schledorn, A.A. Malär, A. Torosyan, S. Penzel, D. Klose, A. Oss, M. Org, S. Wang, L. Lecoq, R. Cadalbert, A. Samoson, A. Böckmann, and B.H. Meier, ChemBioChem **21**, 2540 (2020).
- <sup>5</sup> A. Böckmann, M. Ernst, and B.H. Meier, J. Magn. Reson. **253**, 71 (2015).
- <sup>6</sup> F.D. Doty, EMagRes (2007).
- <sup>7</sup> F.D. Doty and P.D. Ellis, Rev. Sci. Instrum. **52**, 1868 (1981).
- <sup>8</sup> N. Herzog, A. Weber, A. Porea, D. Osen, B. Knott, F. Engelke, and D. Wilhelm, J. Fluids Eng. **144**, (2022).
- <sup>9</sup> K. Xu, O. Pecher, M. Braun, and J. Schmedt auf der Günne, J. Magn. Reson. **333**, (2021).
- <sup>10</sup> D. Banks, B. Michael, N. Golota, and R.G. Griffin, J. Magn. Reson. **335**, 107126 (2022).
- <sup>11</sup> A.B. Barnes, M.L. Mak-Jurkauskas, Y. Matsuki, V.S. Bajaj, P.C.A. van der Wel, R. DeRocher, J. Bryant, J.R. Sirigiri, R.J. Temkin, J. Lugtenburg, J. Herzfeld, and R.G. Griffin, J. Magn. Reson. **198**, 261 (2009).
- <sup>12</sup> J.I. Kelz, J.E. Kelly, and R.W. Martin, J. Magn. Reson. **305**, 89 (2019).
- <sup>13</sup> H. Vanduffel, C. Parra-Cabrera, W. Gsell, R. Oliveira-Silva, L. Goossens, R. Peeters, U. Himmelreich, B. Van Hooreweder, D. Sakellariou, W. Vanduffel, and R. Ameloot, Adv. Mater. Technol. **2200647**, 2200647 (2022).
- <sup>14</sup> J.I. Kelz, J.L. Uribe, and R.W. Martin, J. Magn. Reson. Open **6–7**, 100011 (2021).
- <sup>15</sup> S.J. Elliott, M. Ceillier, O. Cala, Q. Stern, S.F. Cousin, and S. Jannin, J. Magn. Reson. Open **10–11**, 100033 (2022).
- <sup>16</sup> Z. Long, J. Ruthford, and S.J. Opella, J. Magn. Reson. **327**, 106957 (2021).

- <sup>17</sup> F. Ellermann, A. Pravdivtsev, and J.-B. Hövener, *Magn. Reson.* **2**, 49 (2021).
- <sup>18</sup> L. Delage-Laurin, R.S. Palani, N. Golota, M. Mardini, Y. Ouyang, K.O. Tan, T.M. Swager, and R.G. Griffin, *J. Am. Chem. Soc.* **143**, 20281 (2021).
- <sup>19</sup> K.O. Tan, L. Yang, M. Mardini, C.B. Cheong, B. Driesschaert, M. Dincă, and R.G. Griffin, *Chem. – A Eur. J.* **13**, 287 (2022).
- <sup>20</sup> J. Xie, X. You, Y. Huang, Z. Ni, X. Wang, X. Li, C. Yang, D. Zhang, H. Chen, H. Sun, and Z. Chen, *Nat. Commun.* **11**, 1 (2020).
- <sup>21</sup> P. Chen, B.J. Albert, C. Gao, N. Alaniva, L.E. Price, F.J. Scott, E.P. Saliba, E.L. Sesti, P.T. Judge, E.W. Fisher, and A.B. Barnes, *Sci. Adv.* **4**, eaau1540 (2018).
- <sup>22</sup> C. Gao, P.T. Judge, E.L. Sesti, L.E. Price, N. Alaniva, E.P. Saliba, B.J. Albert, N.J. Soper, P.-H. Chen, and A.B. Barnes, *J. Magn. Reson.* (2019).
- <sup>23</sup> H. Furukawa, F. Gándara, Y.-B. Zhang, J. Jiang, W.L. Queen, M.R. Hudson, and O.M. Yaghi, *J. Am. Chem. Soc.* **136**, 4369 (2014).
- <sup>24</sup> D. Wilhelm, A. Porea, and F. Engelke, *J. Magn. Reson.* **257**, 51 (2015).
- <sup>25</sup> N. Herzog, D. Wilhelm, S. Koch, A. Porea, D. Osen, B. Knott, and F. Engelke, *J. Fluids Eng.* **138**, 1 (2016).
- <sup>26</sup> A.E. Bennett, R.G. Griffin, J.H. Ok, and S. Vega, *J. Chem. Phys.* **96**, 8624 (1992).
- <sup>27</sup> S. Devautour-Vinot, G. Maurin, C. Serre, P. Horcajada, D. Paula da Cunha, V. Guillerme, E. de Souza Costa, F. Taulelle, and C. Martineau, *Chem. Mater.* **24**, 2168 (2012).
- <sup>28</sup> M. Hohwy, H.J. Jakobsen, M. Edén, M.H. Levitt, and N.C. Nielsen, *J. Chem. Phys.* **108**, 2686 (1998).
- <sup>29</sup> C.G. Joo, A. Casey, C.J. Turner, and R.G. Griffin, *J. Am. Chem. Soc.* **131**, 12 (2009).
- <sup>30</sup> X.L. Wang, Y.F. Yao, W.C. Qiao, J. Liang, W. Dong, and K. Ma, *J. Phys. Chem. C* **125**, 9908 (2021).
- <sup>31</sup> V.S. Bajaj, M.L. Mak-Jurkauskas, M. Belenky, J. Herzfeld, and R.G. Griffin, *Proc. Natl. Acad.*

Sci. U. S. A. **106**, 9244 (2009).

<sup>32</sup> Q.Z. Ni, T. Van Can, E. Daviso, M. Belenky, R.G. Griffin, and J. Herzfeld, J. Am. Chem. Soc. **140**, 4085 (2018).

<sup>33</sup> S. Xu, W. Zhang, X. Liu, X. Han, and X. Bao, J. Am. Chem. Soc. **131**, 13722 (2009).

<sup>34</sup> M. Hunger, M. Seiler, and T. Horvath, Catal. Letters **57**, 199 (1999).

<sup>35</sup> M. Hunger, T. Horvath, and J. Weitkamp, Stud. Surf. Sci. Catal. **105 B**, 853 (1997).

<sup>36</sup> M. Hunger and T. Horvath, J. Chem. Soc. Chem. Commun. 1423 (1995).

<sup>37</sup> P. Berruyer, S. Björgvinsdóttir, A. Bertarelli, G. Stevanato, Y. Rao, G. Karthikeyan, G. Casano, O. Ouari, M. Lelli, C. Reiter, F. Engelke, and L. Emsley, J. Phys. Chem. Lett. **11**, 8386 (2020).


<sup>38</sup> E. Barbet-Massin, A.J. Pell, J.S. Retel, L.B. Andreas, K. Jaudzems, W.T. Franks, A.J. Nieuwkoop, M. Hiller, V. Higman, P. Guerry, A. Bertarelli, M.J. Knight, M. Felletti, T. Le Marchand, S. Kotelovica, I. Akopjana, K. Tars, M. Stoppini, V. Bellotti, M. Bolognesi, S. Ricagno, J.J. Chou, R.G. Griffin, H. Oschkinat, A. Lesage, L. Emsley, T. Herrmann, and G. Pintacuda, J. Am. Chem. Soc. **136**, 12489 (2014).

<sup>39</sup> J. Cui, J. Li, X. Peng, and R. Fu, J. Magn. Reson. **284**, 73 (2017).

# Supporting Information

## Design and Fabrication of Cap Removal Tool via CNC Machining

We have designed and fabricated a cap-removal tool (**Fig. S1**) for a 7 mm rotor system. The tool was designed on Autodesk Inventor (see supplementary data for the model), and it can be easily adapted for any rotor sizes. The tool consists of only two pieces, which were held together with a screw and a nut. We used Fusion360 as the Computer-Aided Manufacturing (CAM) software for simulating the toolpath. The g-code is later loaded into the Grbl software, which guides the CNC machine (Genmitsu PROVerXL 4030). We machined the cap-removal tool on a 5 mm aluminum sheet using a 3 mm titanium nitride (TiN) coated end mill loaded to an ER 11 collet on a 300 W spindle capable of spinning up to 10,000 rpm. The manufacturing time was ~ 3 hr per piece, and it has successfully removed several drive caps from the 7 mm rotor.

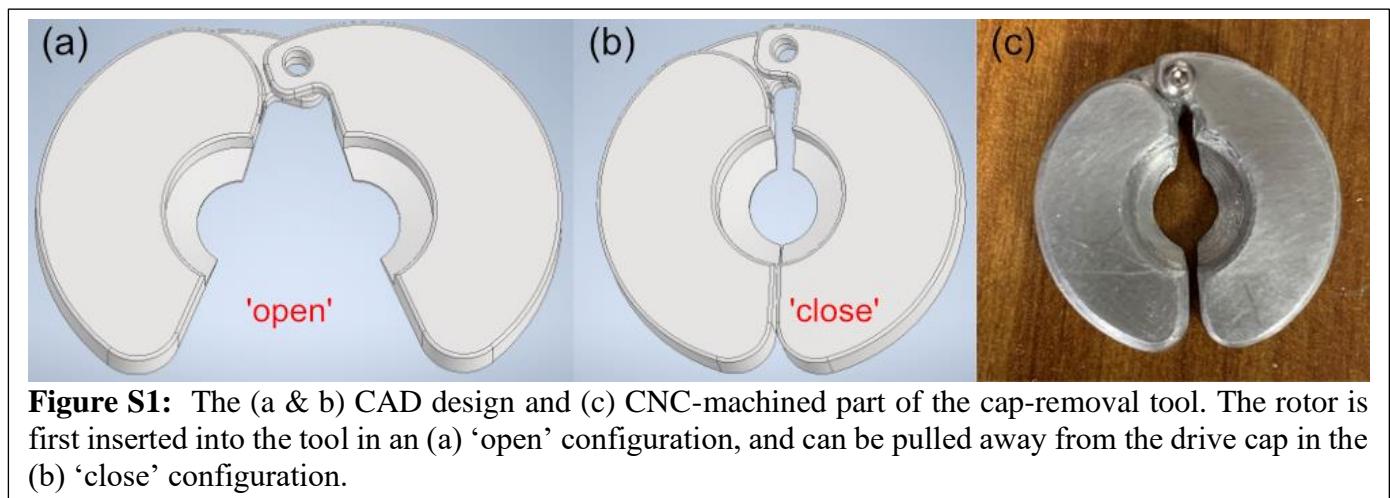

**Figure S1:** The (a & b) CAD design and (c) CNC-machined part of the cap-removal tool. The rotor is first inserted into the tool in an (a) 'open' configuration, and can be pulled away from the drive cap in the (b) 'close' configuration.

## Design of MAS Drive Caps

We have included the '\*.ipt' (Autodesk Inventor) '\*.stl' files for the 1.3, 2.5, 3.2, 4, and 7-mm drive caps, as well as the cap-removal tool for the 7 mm system (adaptable to other dimensions). Note that the dimensions of all drive caps were reiteratively optimized to be printed using Clear V4 resins and Form 3+ (Formlabs), except the 4 mm, which was printed using Elegoo Saturn. Moreover, note that the shape of the slab in the 2.5 mm cap and the fins of the 1.3 mm were also optimized for better MAS performances. Note that the shape of the printed parts depends on the ambient environment surrounding the 3D printer, i.e., temperature, ambient light condition, etc. Hence, some minor alterations to the design might be necessary to yield satisfactory results.