


Test Procedure Reference	Calibration	Job No.	Calibration
Unique No.	Calibration	Test Description	Calibration
R&D Reference	Calibration	Test Date	01/10/2025
Valve Description	Calibration	Valve Drawing No.	Calibration



Calibration BX Port

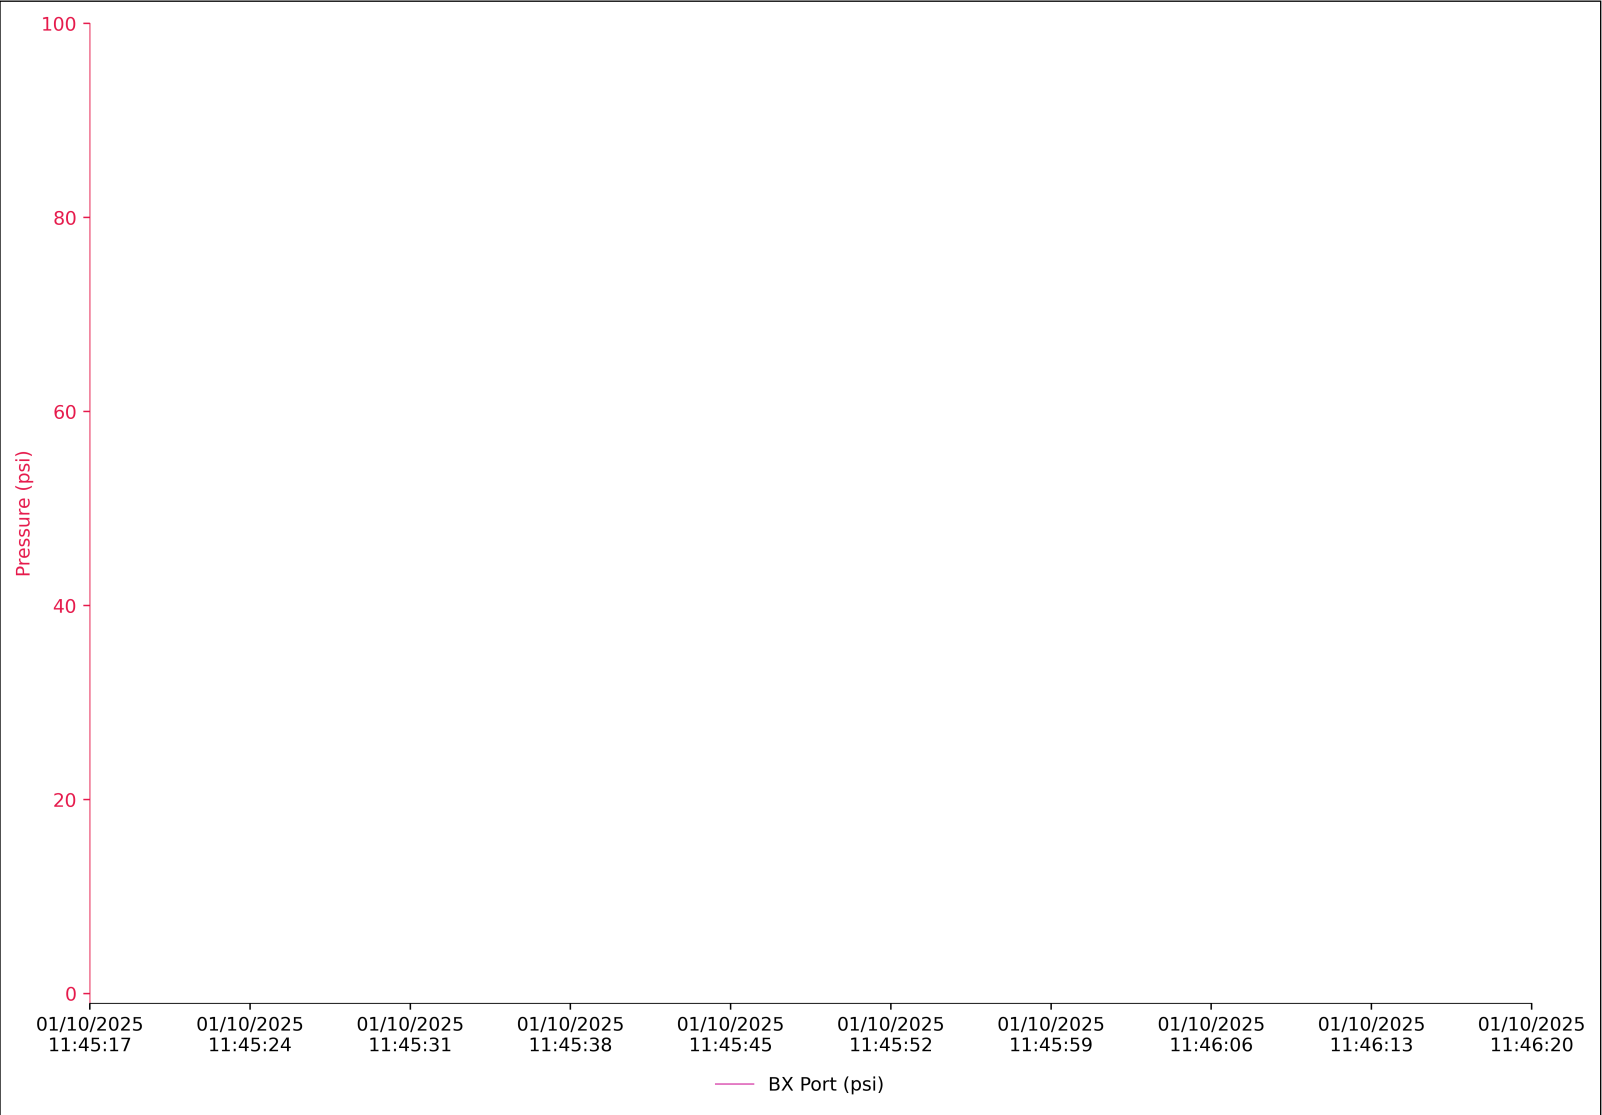

Applied (µA)	4000.0	8000.0	12000.0	16000.0	20000.0
Counts (avg)	-1960523	-1960522.0	-1960519.0	-1960524.0	-1960526.0
Converted (µA)	-15.151	-15.148	-15.143	-15.152	-15.158
Abs Error (µA) - ±3.6 µA	4015.15	8015.15	12015.14	16015.15	20015.16

Data Recording Equipment Used

Data Logger	Right Hand Large Temperature
Serial No.	8a7d5ef052b47810
Transducers	

Gauges

Torque Transducer N/A

Cycle Count	1
-------------	---

Test Pressure	0 psi
---------------	-------

Breakout Torque	N/A
Running Torque	N/A

Coefficient	Value
S3	-0.067883
S2	-1.3309e+05
S1	2.6091e+11
S0	5.1152e+17

3rd Party Stamp and Date

Operative: Toby Lelean