


Test Procedure Reference	Calibration	Job No.	Calibration
Unique No.	Calibration	Test Description	Calibration
R&D Reference	Calibration	Test Date	10/09/2025
Valve Description	Calibration	Valve Drawing No.	Calibration



Calibration Upstream

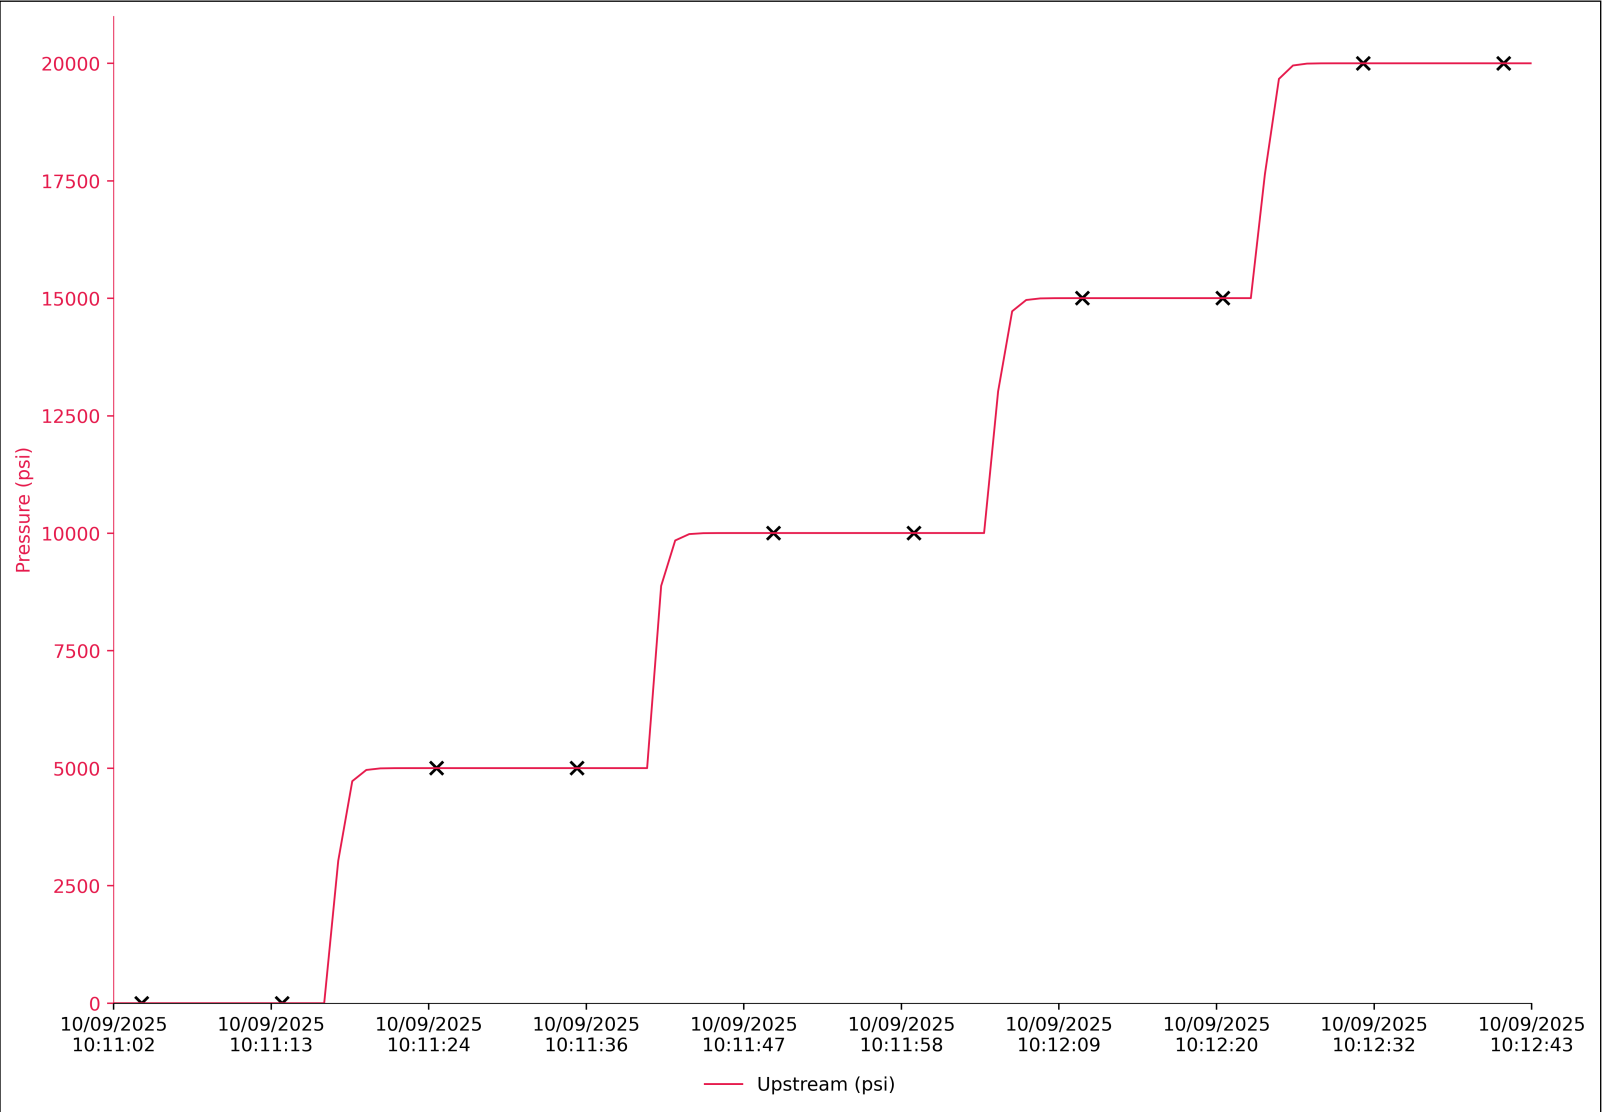

Data Recording Equipment Used

Data Logger DLS Prototype  
Serial No. N/A  
Transducers

Gauges

Torque Transducer N/A

Cycle Count 1

Test Pressure 0 psi

Breakout Torque N/A

Running Torque N/A

	1	2	3	4	5
	nan	nan	nan	nan	nan
Measured	0.0	5003.0	10005.0	15004.0	20001.0
Expected	0.0	5000.0	10000.0	15000.0	20000.0
Error %	0.0	0.06	0.05	0.027	0.005

3rd Party Stamp and Date

Operative: Jason Bradley