
Shift/Outlier Analysis– Maximum During Baseline to Maximum During Post-baseline for Lab test 1
Population xxxx

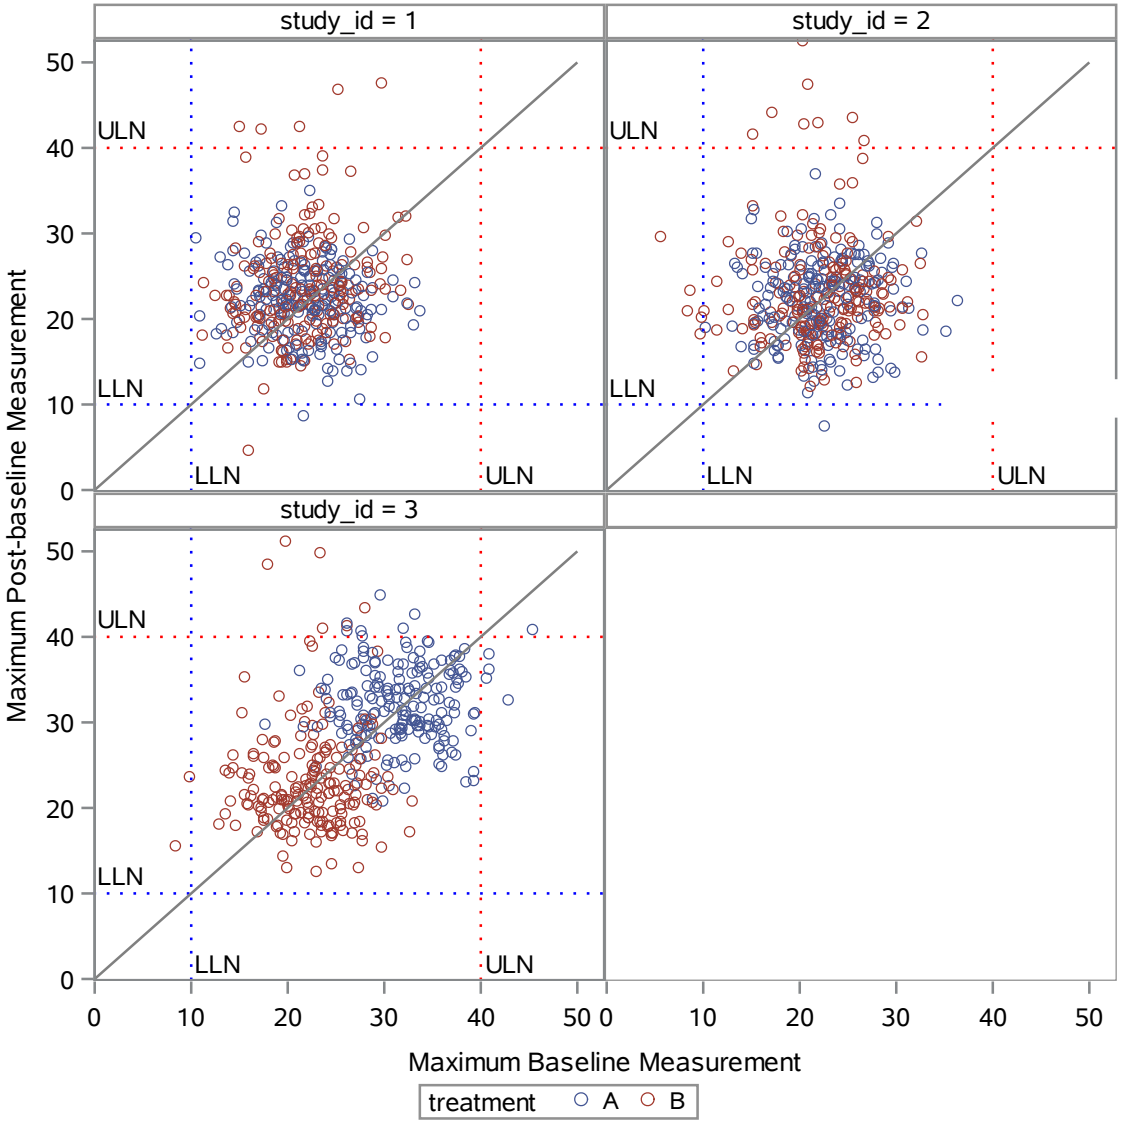

Treatment Emergent High

Treatment	N	n	%
A	600	30	5.0
B	600	45	7.5

Treatment Comparison - B vs. A

MH Odds Ratio	Heterogenity P value	CMH P value
1.54	0.238	0.324

N=number o…eline measurement below upper…e post-baseline measurement; n = number of subjects with a post-baseline measurement above upper limit of normal; CMH P-value = Cochran-Mantel-Haenszel (CMH) test stratified by study.
The denominator for Mantel-Haenszel odds ratio is treatment A
Heterogeneity P value is from Breslow-Day test.

XXX lab reference range is used.