


Two-year windows: controlled timing diagnostic

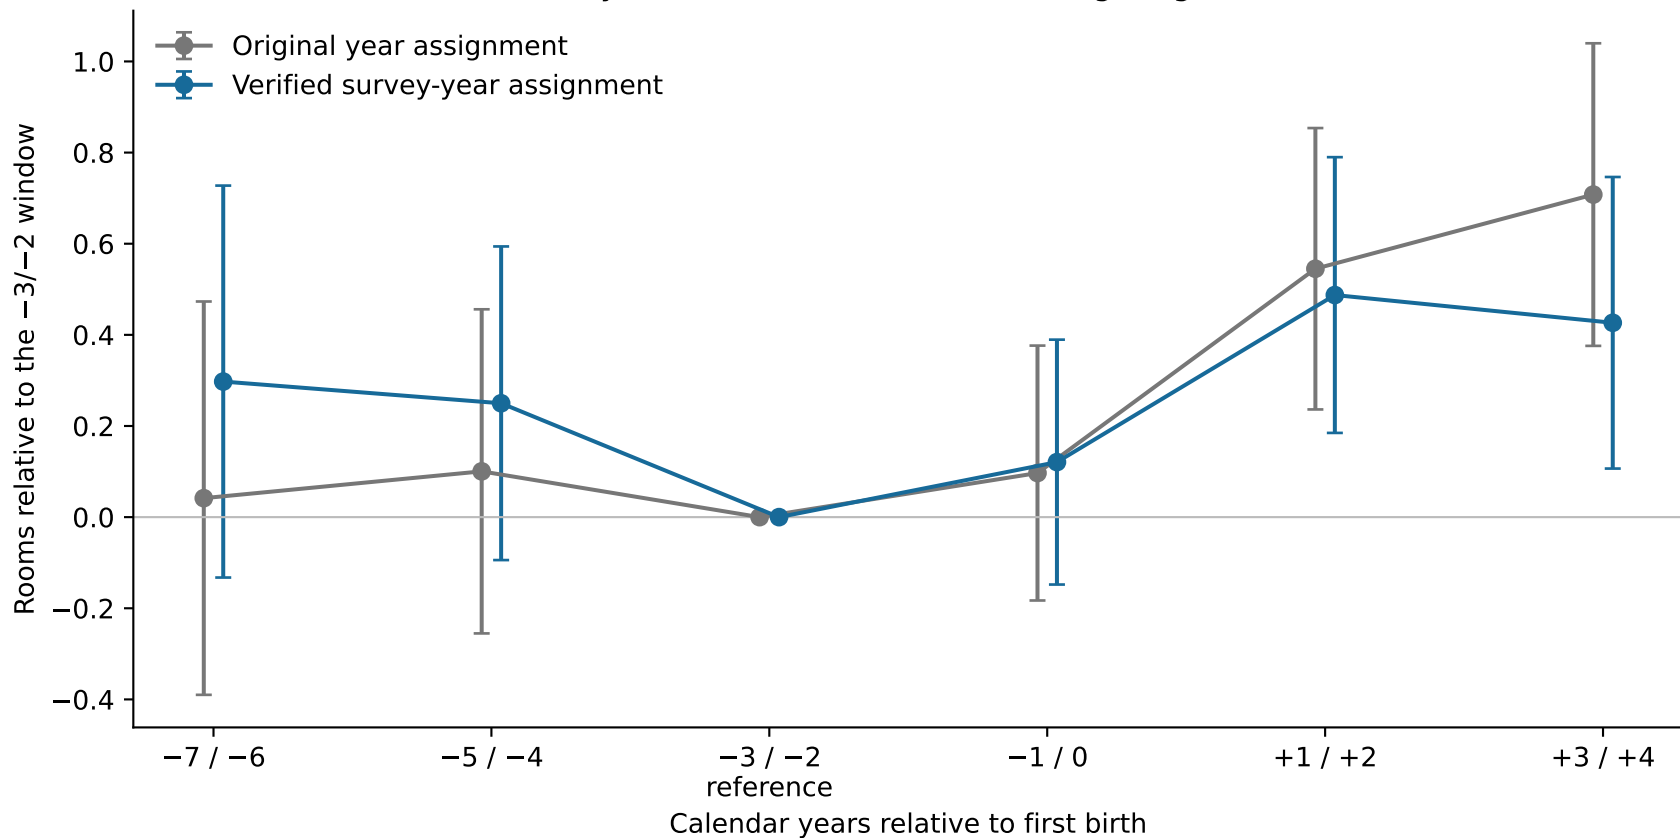

Same sample and supported birth cohorts; individual/year FE; unweighted.
2019 comparison cohort used only before 2019. Original room codes retained. Diagnostic, not a new calibration target.