

Resistive-pulse sensing at the micro- and nanoscale

Preston Hinkle




University of
California, Irvine

August 15, 2017

Outline



- Resistive pulse sensing background
- Resistive pulse sensing of high-aspect ratio particles
- Microscale resistive pulse sensing
 - Simultaneous imaging and resistive pulse studies
 - Cancer cell deformability cytometry

Oct. 20, 1953 W. H. COULTER 2,656,508
MEANS FOR COUNTING PARTICLES SUSPENDED IN A FLUID
Filed Aug. 27, 1949
2 Sheets-Sheet 1

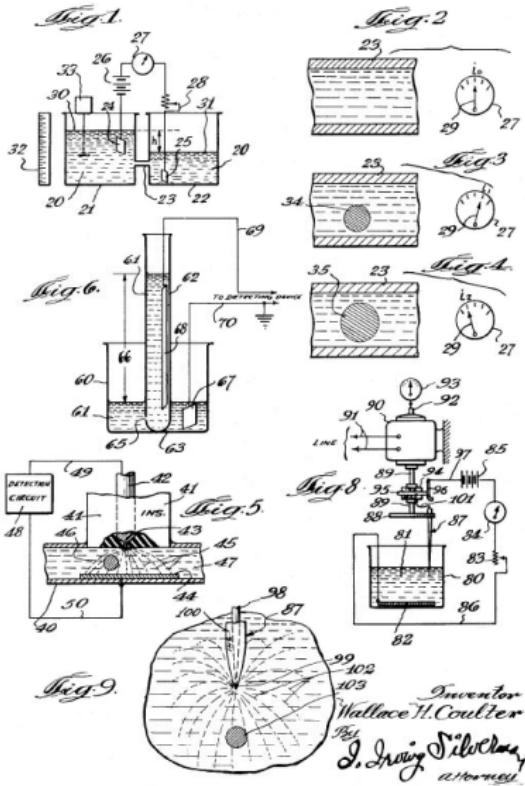


Outline

- Resistive pulse sensing background
- Resistive pulse sensing of high-aspect ratio particles
- Microscale resistive pulse sensing
 - Simultaneous imaging and resistive pulse studies
 - Cancer cell deformability cytometry

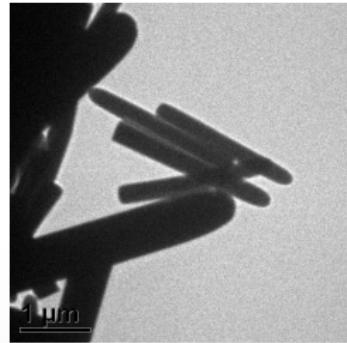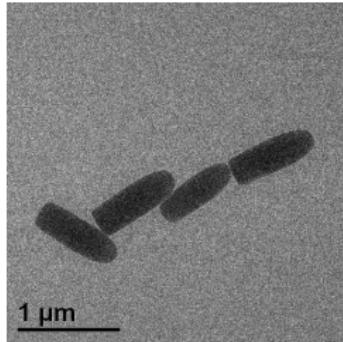


Outline

- Resistive pulse sensing background
- Resistive pulse sensing of high-aspect ratio particles
- Microscale resistive pulse sensing
 - Simultaneous imaging and resistive pulse studies
 - Cancer cell deformability cytometry

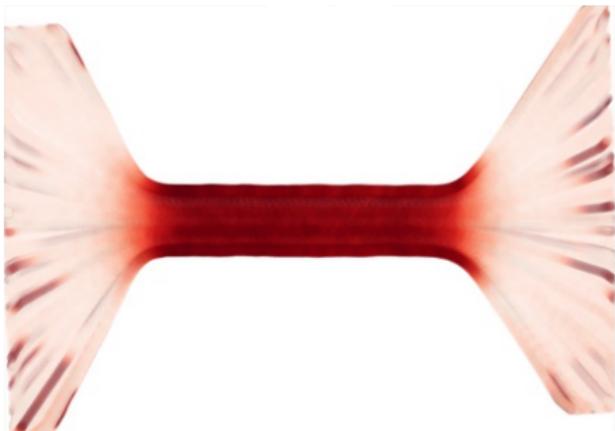

Outline


- Resistive pulse sensing background
- Resistive pulse sensing of high-aspect ratio particles
- Microscale resistive pulse sensing
 - Simultaneous imaging and resistive pulse studies
 - Cancer cell deformability cytometry

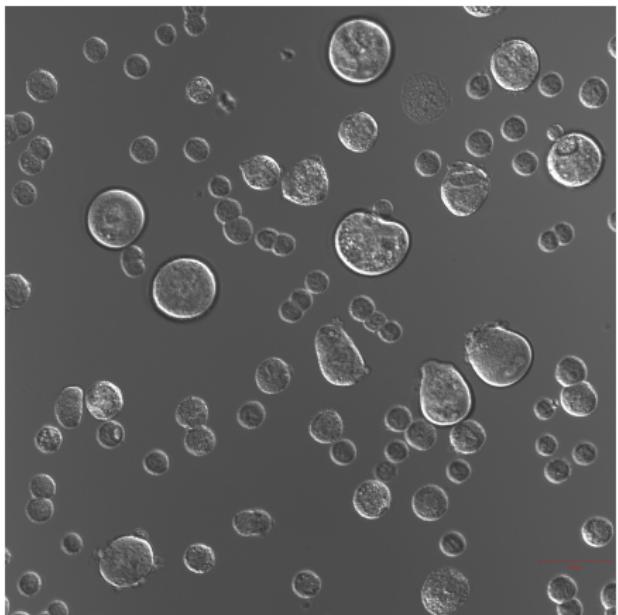

Resistive pulse sensing background



Resistive pulse sensing—description

- Resistive pulse sensing (RP) is a method for single particle detection and characterization
- Works at any scale (nano, micro, milli, etc.)
- A diverse range of applications: red blood cell counting (several μm , virus detection (10 – 100 μm , and DNA sequencing ($\sim 1 \text{ nm}$), among others

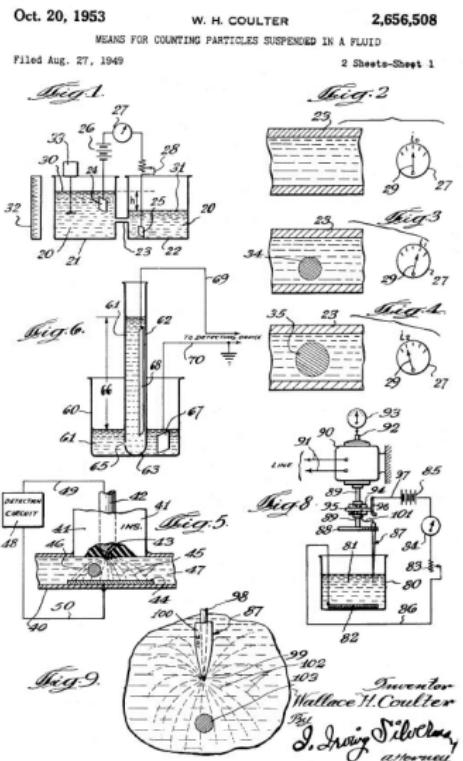


Resistive pulse sensing—how does it work?


- A nanopore immersed in electrolyte solution acts as an ionic resistor
- Current-Voltage relationship follows Ohm's law $V = IR$
- When a particle enters the channel its resistance changes, yielding a pulse in the measured ionic current
- Pulse properties yield information on size, shape, charge, and concentration of particle

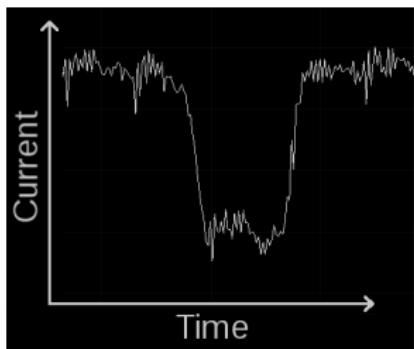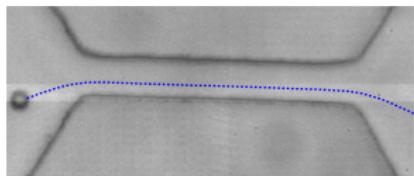

Resistive pulse sensing—system components

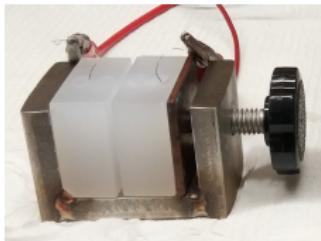


Conductivity cell



Pore membrane



Electrolyte



Particles




Ag-AgCl
electrodes




Voltage amplifier + current recorder

Resistive pulse sensing

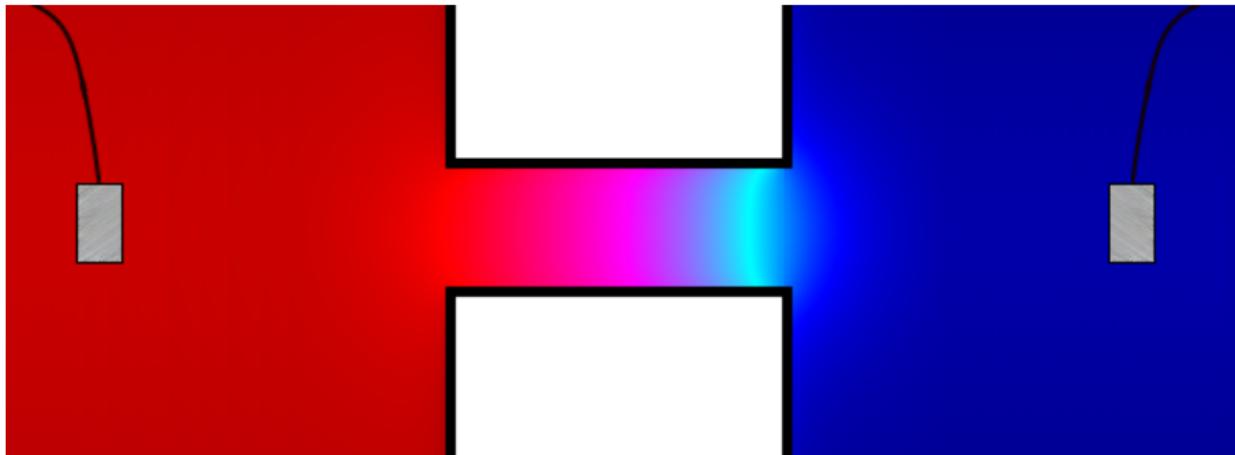

Resistive pulse sensing—electrostatic boundary conditions

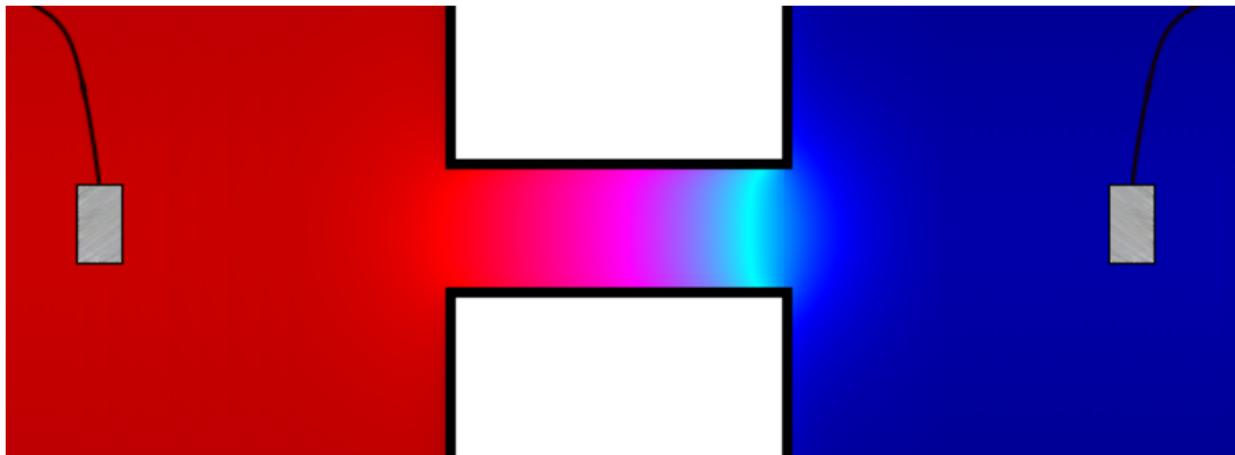

Resistive pulse sensing—ion transport

- Ion transport is driven by **diffusion**, **convection**, and **electric migration**
- Diffusion: Average flow of ions from high to low concentration
- Convection: Ions move with the fluid/solvent
- Electrical migration: Ions move in electric field

$$\vec{J}_i = \underbrace{z_i e D_i \nabla c_i}_{\text{diffusion}} + \overbrace{z_i e c_i \vec{u}}^{\text{convection}} + \underbrace{z_i e c_i \mu_i \vec{E}}_{\text{migration}}$$

$$I = \sum_i \iint_S \vec{J}_i \cdot \hat{n} dS$$

Resistive pulse sensing—ion transport

- Ion transport is driven by **diffusion**, **convection**, and **electric migration**
- Diffusion: Average flow of ions from high to low concentration
- Convection: Ions move with the fluid/solvent
- Electrical migration: Ions move in electric field



$$\vec{J}_i = \underbrace{z_i e D_i \nabla c_i}_{\text{diffusion}} + \underbrace{z_i e c_i \vec{u}}_{\text{convection}} + \underbrace{z_i e c_i \mu_i \vec{E}}_{\text{migration}}$$

$$I = \sum_i \iint_S \vec{J}_i \cdot \hat{n} dS$$

Resistive pulse sensing of high-aspect ratio particles

High-aspect ratio resistive pulse sensing—motivation

- Aspherical particles are ubiquitous in biology—e.g., viruses, bacteria
- RP sensing allows volume determination
- Can we extend RP to measure length?
- How would we do so?

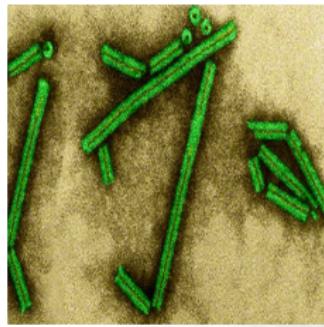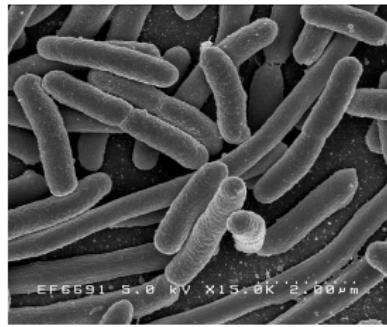


Resistive pulse in non-constant width pores

- Change in resistance of pore is approximately



$$\Delta R(z') = \frac{\rho}{\pi} \int_{z=z'}^{z=z'+l_p} \frac{dz}{r_p^2(z) - s_p^2(z)}$$

- RP amplitude is a function of the pore geometry **local to the particle's position**
- Particles map the interior of the pore during translocation with their RP signal!

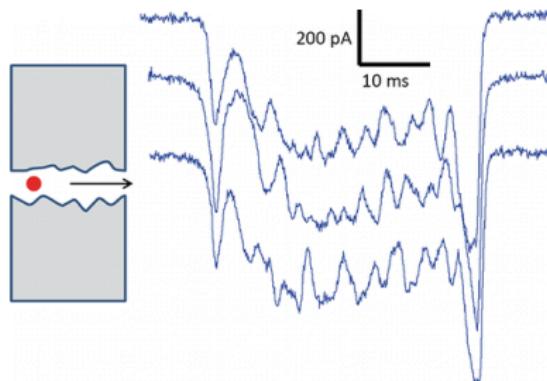

Resistive pulse in non-constant width pores

- For particles with length shorter than characteristic length of changes in pore size, the interior is mapped with high resolution
- Long particles map pore interiors with low resolution because their lengths extend along multiple features

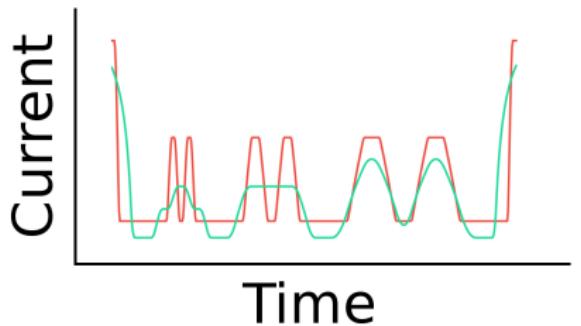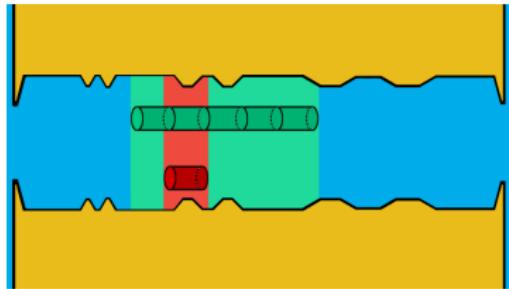

Length measurement experimental platform

- Resistive pulses can be seen as a map of the pore interior for pores with non-constant radius
- In regions of low diameter, the pulse is deeper; in large diameter regions, the pulse is shallow
- Particles shorter than the length scale of diameter variation accurately map the pore interiors
- Particles longer than the length scale of diameter variation create RP signals that can be seen as a convolution of the pore's interior shape

$$\begin{aligned}\Delta R = R_p - R_0 &= \rho \int_{z=0}^{z=l_p} \frac{dz}{A(z)} - \rho \int_{z=0}^{z=l_p} \frac{dz}{A'(z)} \\ &= \rho \int_{z=z'-l_p/2}^{z=z'+l_p/2} \frac{1}{\pi [r_p^2(z) - r_p^2(z')]} - \frac{1}{\pi r_p^2(z)}\end{aligned}\tag{1}$$