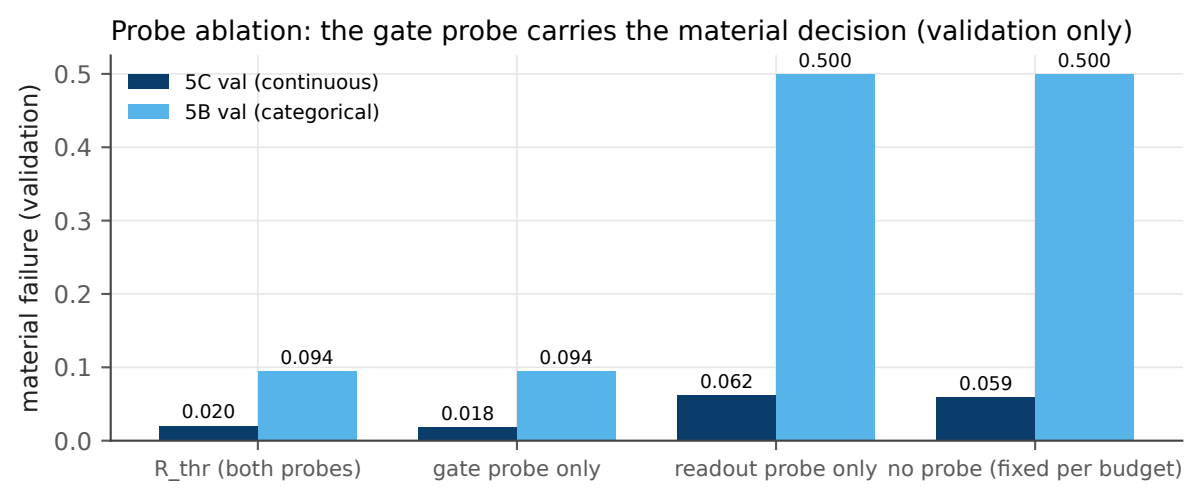
Probe ablation: the gate probe carries the material decision (validation only)
material failure (validation)
0.5
0.4
0.3
0.2
0.1
0.0
5C val (continuous)
5B val (categorical)
0.020
0.094
0.018
0.094
0.062
0.500
0.059
0.500
R_thr (both probes)
gate probe only
readout probe only
no probe (fixed per budget)