

DLS Analysis Report

June 9, 2026

Experiment Metadata

Analysis started	2026-06-09 16:57:32
JADE-DLS version	2.0
Angles	30ř, 40ř, 50ř, 60ř, 70ř, 80ř, 90ř, 100ř, 110ř, 120ř, 130ř, 140ř, 150ř
Temperature	297.94 ± 0.005 K
Viscosity	0.8945 cP
Files	39

Result Details — Method A

2026-06-09 16:59:42

Fit	Rh [nm]	Rh error [nm]	D [m ² /s]	std err D [m ² /s]	R _s
Rh from 1st order cumulant fit	80.1057	0.5473	3.046e-12	2.081e-14	0.998
Rh from 2nd order cumulant fit	78.3628	0.4530	3.113e-12	1.800e-14	0.998
Rh from 3rd order cumulant fit	78.3585	0.4674	3.114e-12	1.857e-14	0.998
Order	Slope (DCE10ž mš/s)	Std Error	Rš	Quality	
1st	3045.730080	20.809402	0.998276	Excellent	
2nd	3113.470797	17.998126	0.998765	Excellent	
3rd	3113.643288	18.571764	0.998685	Excellent	

Result Details — Method C

2026-06-09 16:59:51

Rh [nm]	Rh error [nm]	D [mš/s]	D error [mš/s]	R _{squared}	Fit
78.5425	0.5355	3.106e-12	2.118e-14	0.9983	Rh from iterative non-linear
Model Statistics					
R-squared		0.998283			
Adj. R-squared		0.998237			
F-statistic		2.152e+04			
Prob (F-statistic)		9.046e-53			
AIC		368.51			
BIC		371.83			

Coefficient	Value	Std Error			
Metric	Value	Optimal Range	Assessment		
Rš	0.9983	> 0.95 (Excellent)0.90-0.95 (Acceptable)< 0.90 (Poor)	Excellent		
Adjusted Rš	0.9982	> 0.95 (Excellent)0.90-0.95 (Acceptable)< 0.90 (Poor)	Excellent		
F-statistic	21517.77	> 100 (Excellent)10-100 (Acceptable)< 10 (Poor)	Excellent		
p-value (F-test)	9.046e-53	< 0.001 (Excellent)0.001-0.05 (Acceptable)> 0.05 (Poor)	Excellent		
Moment	Value	Formula	Available for		
Skewness	-5.6345	/ $\wedge(3/2)$	3rd & 4th order		
Kurtosis	-77.5288	/ š	4th order only		
Rh [nm]	Rh error [nm]	D [mš/s]	D error [mš/s]	R_squared	Fit
78.5425	0.5355	3.106e-12	2.118e-14	0.9983	Rh from iterative non-linear
Model Statistics					
R-squared	0.998283				
Adj. R-squared	0.998237				
F-statistic	2.152e+04				
Prob (F-statistic)	9.046e-53				
AIC	368.51				
BIC	371.83				
Coefficient	Value	Std Error			
Metric	Value	Optimal Range	Assessment		
Rš	0.9983	> 0.95 (Excellent)0.90-0.95 (Acceptable)< 0.90 (Poor)	Excellent		
Adjusted Rš	0.9982	> 0.95 (Excellent)0.90-0.95 (Acceptable)< 0.90 (Poor)	Excellent		
F-statistic	21517.77	> 100 (Excellent)10-100 (Acceptable)< 10 (Poor)	Excellent		
p-value (F-test)	9.046e-53	< 0.001 (Excellent)0.001-0.05 (Acceptable)> 0.05 (Poor)	Excellent		
Moment	Value	Formula	Available for		
Skewness	-5.6345	/ $\wedge(3/2)$	3rd & 4th order		
Kurtosis	-77.5288	/ š	4th order only		

Result Summary — Method C

2026-06-09 16:59:55	Method	Rh (nm)	Error (nm)	D (mš/s)	D e
	Method C filtered (N=27 pts, 4th order)	78.28	0.61	3.117e-12	2.42

Result Summary — NNLS Analysis

2026-06-09 17:00:42	Method	Rh (nm)	Error (nm)	D (mš/s)	D err (mš/s)	Rš	PDI
	NNLS Peak 1	75.39	1.17	nan	nan	0.9912	N/A

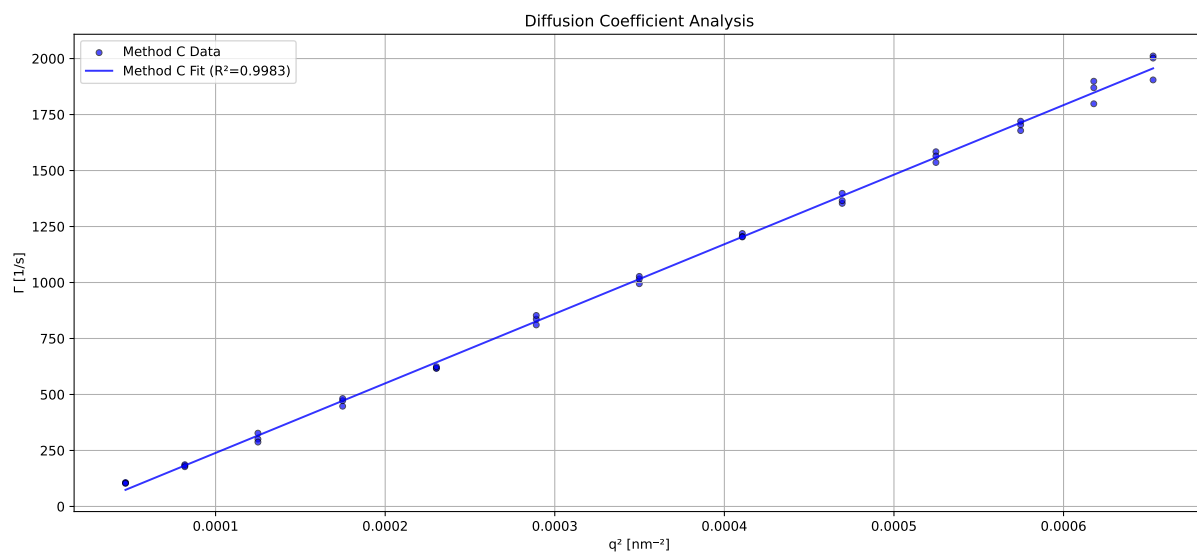


Figure 1: 1. Method C Summary

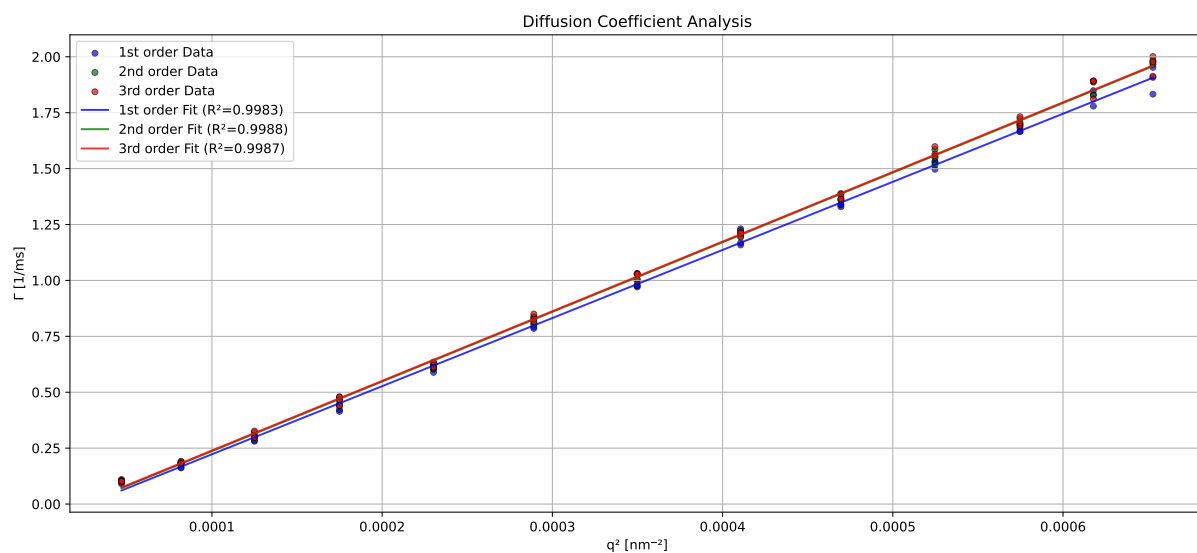


Figure 2: 1. Method A Summary

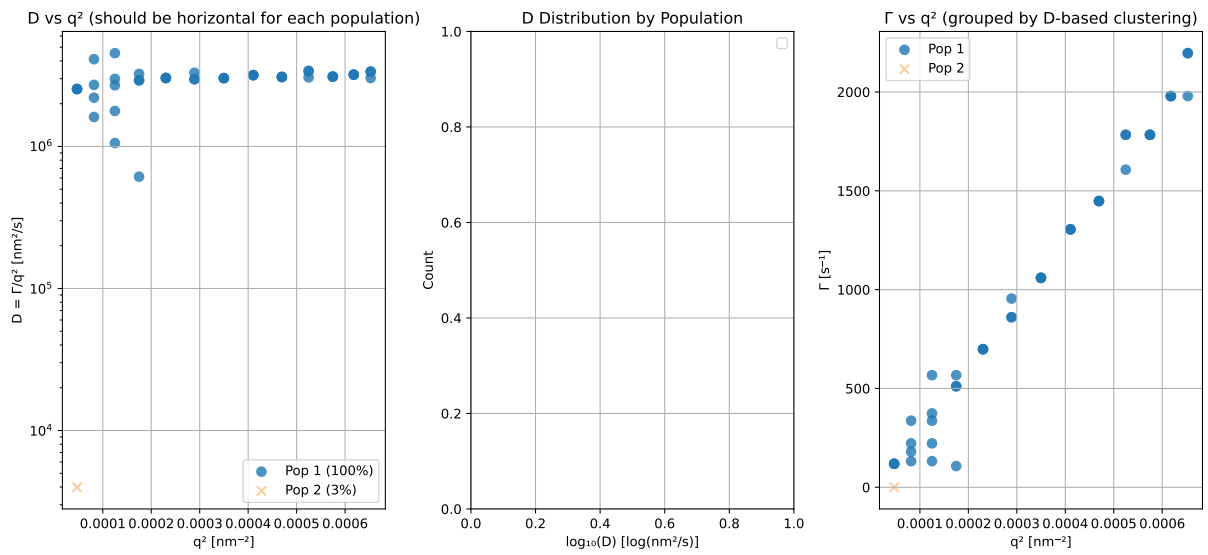


Figure 3: 43. NNLS Peak Clustering