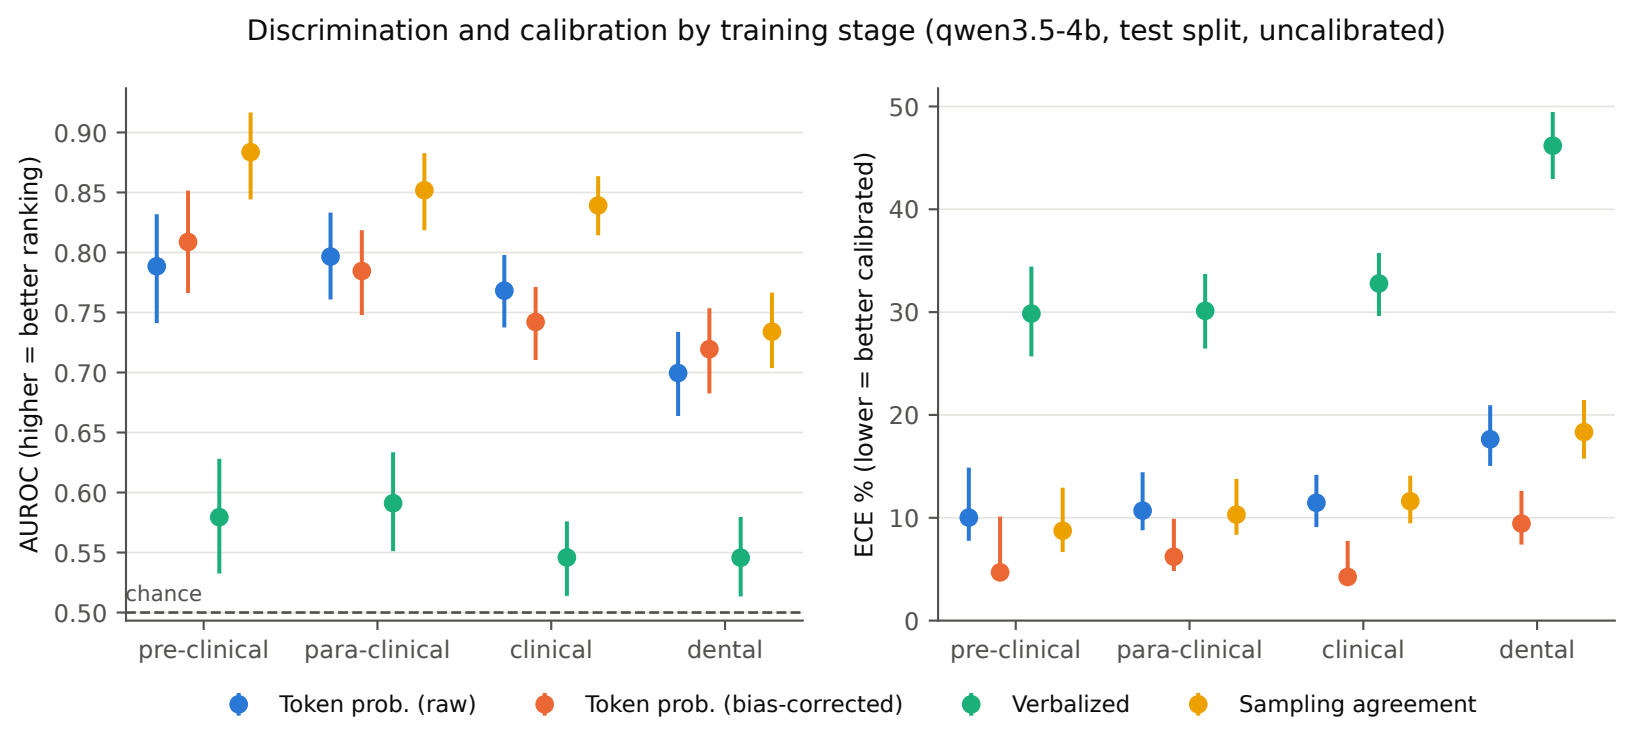
Discrimination and calibration by training stage (qwen3.5-4b, test split, uncalibrated)
AUROC (higher = better ranking)
0.90
0.85
0.80
0.75
0.70
0.65
0.60
0.55
0.50
chance
pre-clinical
para-clinical
clinical
dental
ECE % (lower = better calibrated)
50
40
30
20
10
0
pre-clinical
para-clinical
clinical
dental
Token prob. (raw)
Token prob. (bias-corrected)
Verbalized
Sampling agreement