


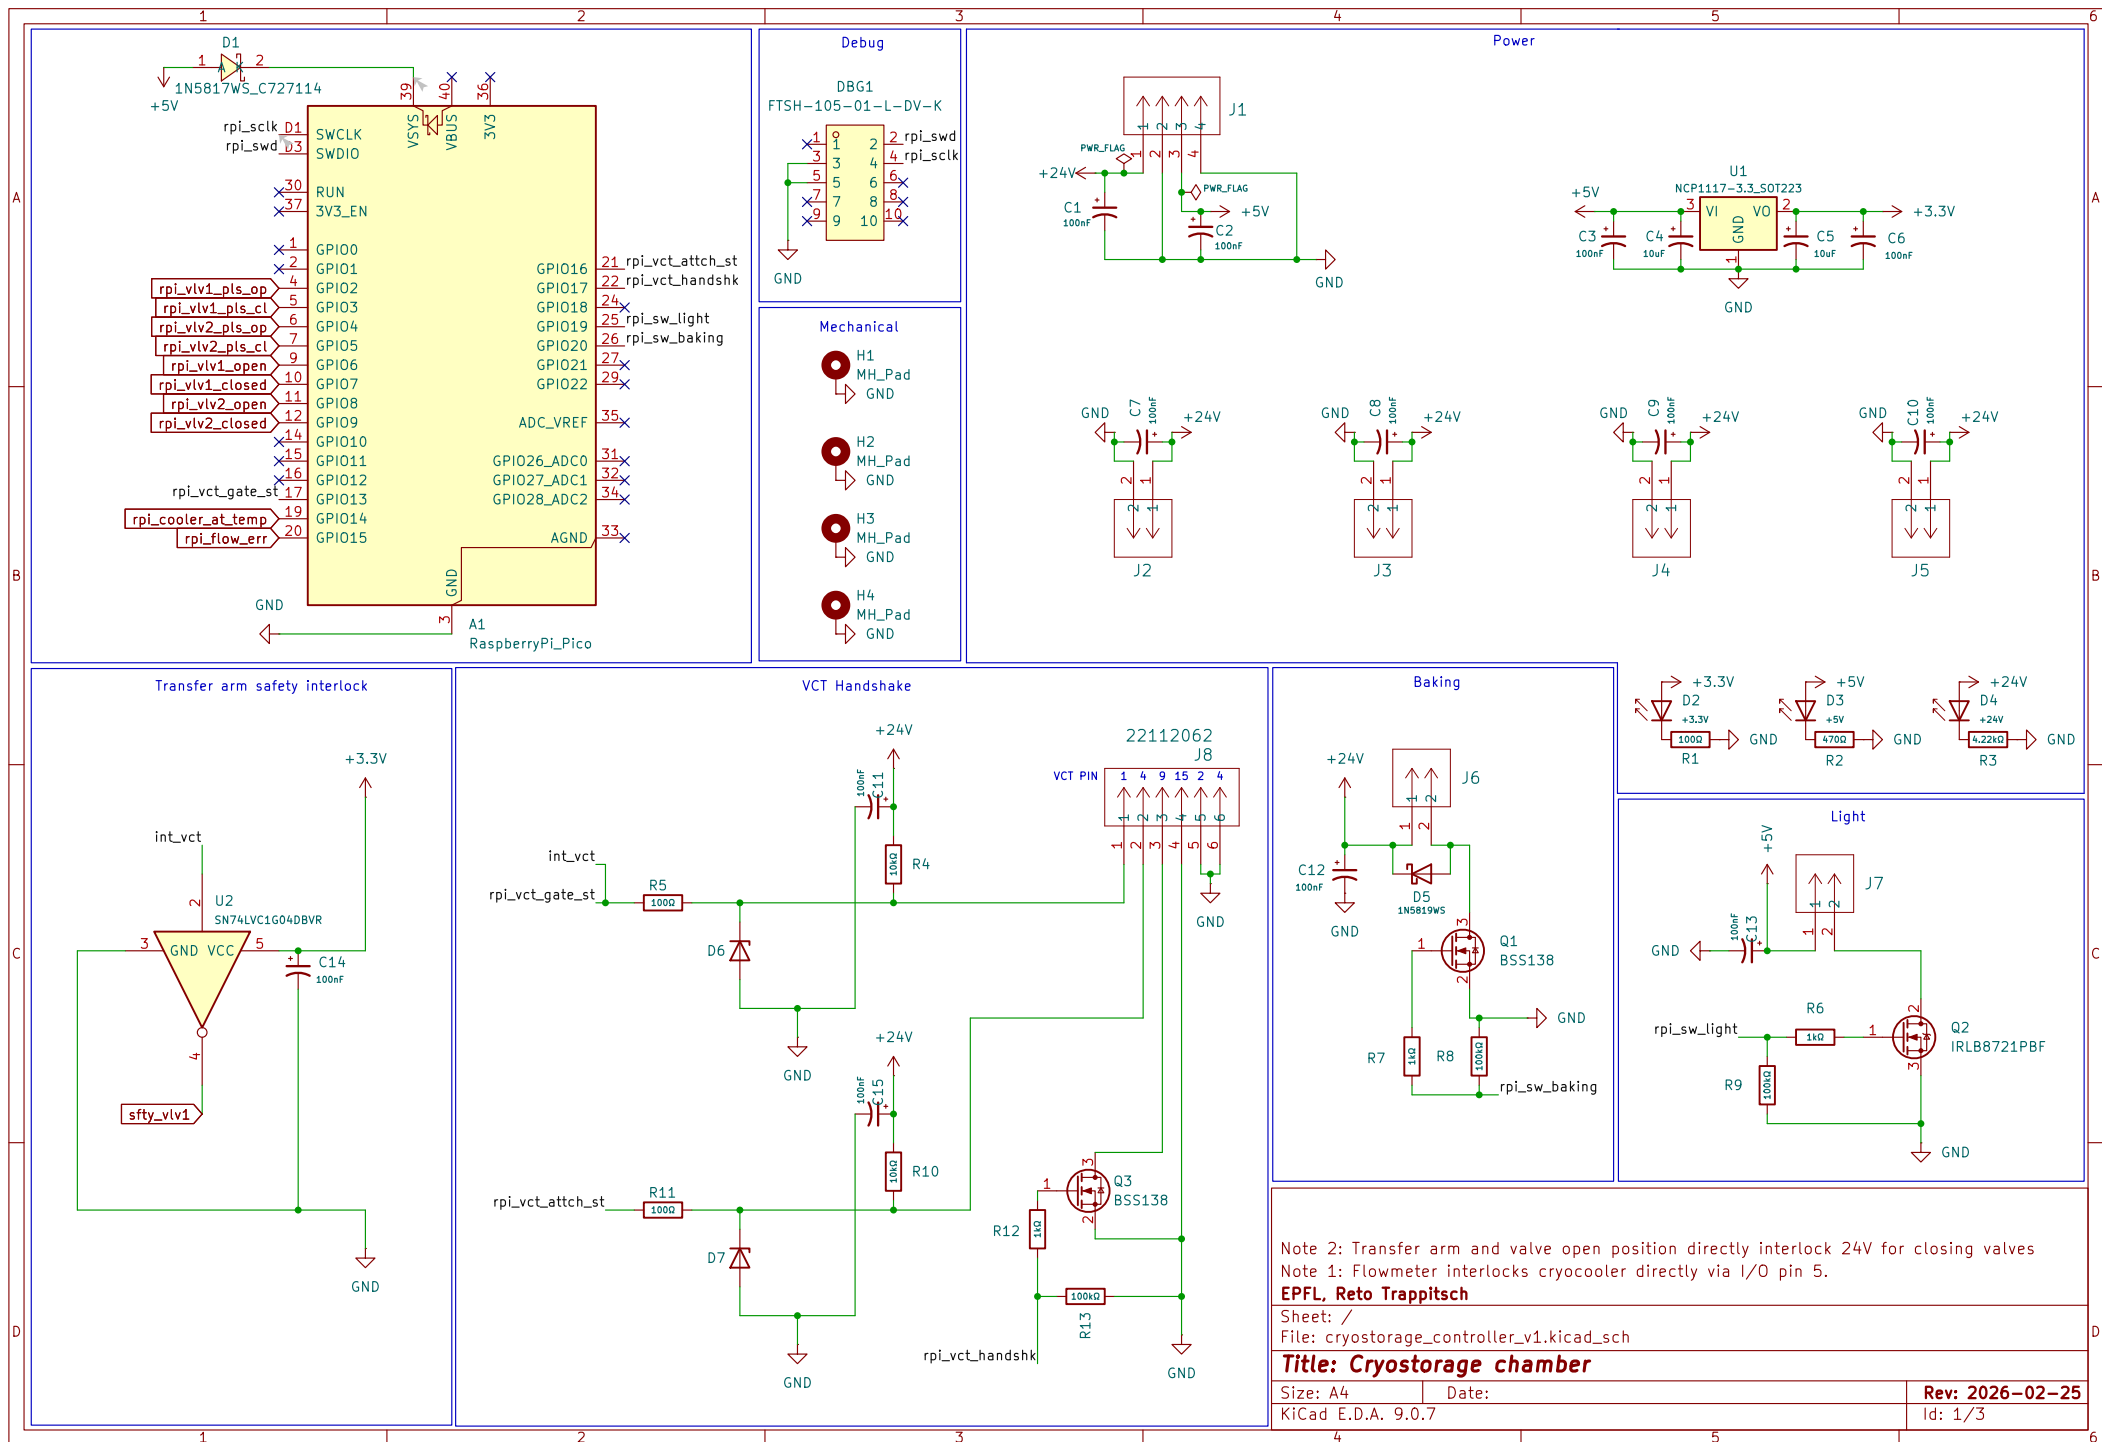

Note 2: Transfer arm and valve open position directly interlock 24V for closing valves
 Note 1: Flowmeter interlocks cryocooler directly via I/O pin 5.

EPFL, Reto Trappitsch

Sheet: /

File: cryostorage_controller_v1.kicad_sch

Title: Cryostorage chamber

Size: A4





Date:

Rev: 2026-02-25

KiCad E.D.A. 9.0.7

Id: 1/3

Gate valves Left: Valve1 (transfer) / Right: Valve2 (pump)

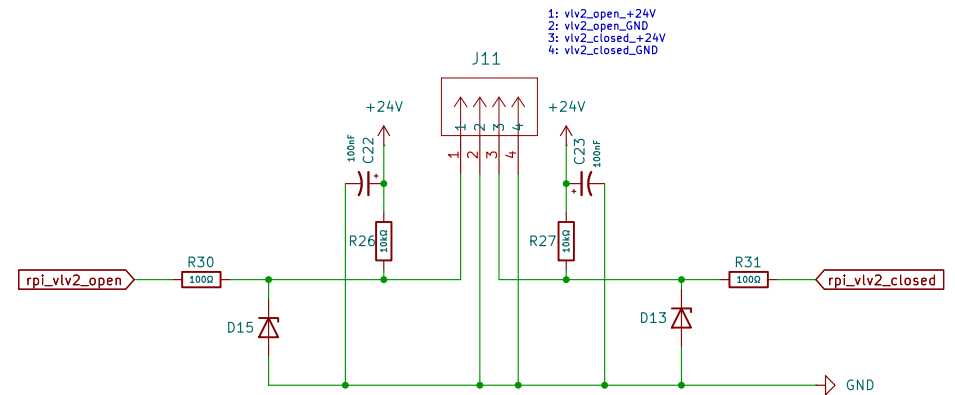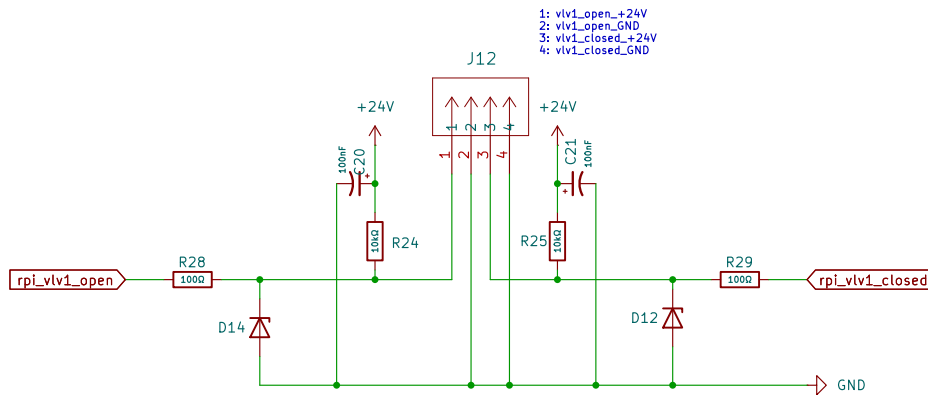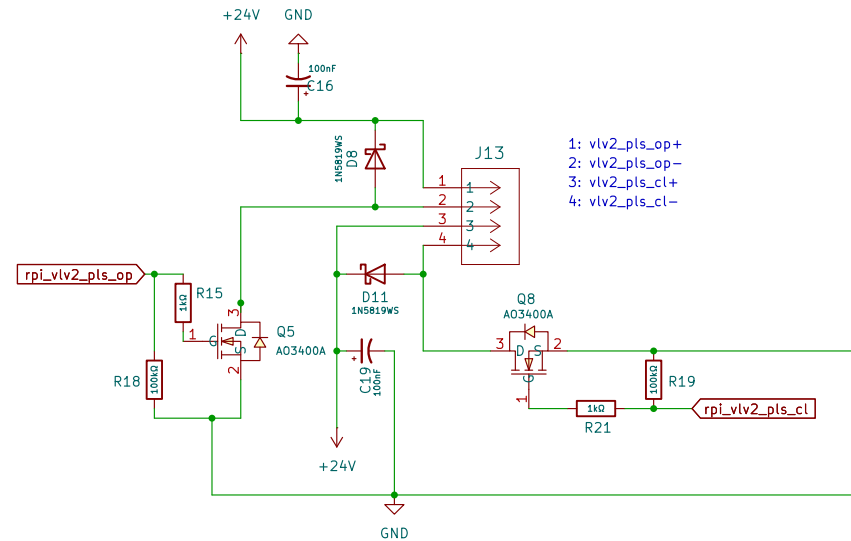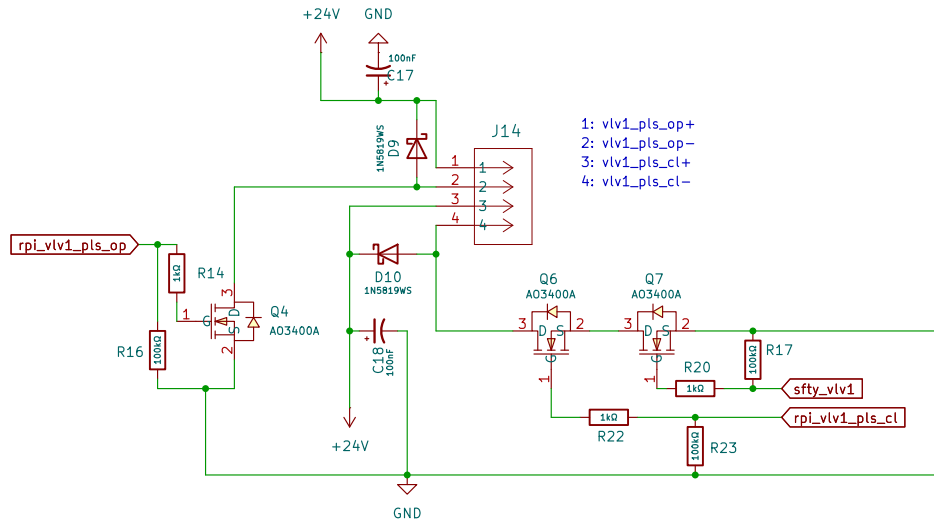

Note 2: Transfer arm and valve open position directly interlock 24V for closing valves

EPFL, Reto Trappitsch

Sheet: /gate_valves/

File: gate_valves.kicad_sch

Title: Cryostorage chamber – Gate valve control

Size: A4

Date:

Rev: 2026-02-25

KiCad E.D.A. 9.0.7

Id: 2/3

