

General

Name of Run	230721_Channel3R1.run	Name of Analysis	TKN_2.ANL
Date of Report	7/24/2023	System	AA500
Run Start	7/21/2023 2:41:55 PM	Run Stop	5:00:37 PM
Operator Run/Rec.	CLMR / CLMR	Software Version	AACE 8.02 SP2
Comment	Recalculate from Run230721_Channel3.run		

Parameters

Channel	3
Method	TKN
Unit	mg/L
Calib. Fit	Slope only
Corr.Coeff.(r)	0.9966
AUFS/Gain	0.13/75
Offset	-2894
Sensitivity	0.1062
Sample Limit 1	-
Sample Limit 2	-

Results

Pk	Cup	Type	Sample ID	Value	Value	Value
0	0	B	Initial Base	0.000		
1	921	P	Primer	2.276		
2	921	D	Drift	2.401		
3	921	C	2.24	2.379		
4	901	C	1.68	1.798		
5	902	C	1.12	1.205		
6	903	C	0.56	0.617		
7	904	C	0.224	0.254		
8	905	C	Blank (SamplerWash)	0.234		
9	0	B	Baseline	0.000		
10	921	H1	High	2.495		
11	904	L1	Low	0.246		
12	904	L1	Low	0.247		
13	905	S	Blank	0.220		
14	906	K	Blank spiked	0.244		
15	907	QC1	CRM (0.8mg/L)	0.216		
16	1	S	1a	0.275		
17	2	S	1	0.339		
18	3	S	3	0.474		
19	4	S	4	0.454		
20	5	S	5	0.136		
21	6	S	6	0.531		
22	7	S	20	0.469		
23	8	S	22	0.389		
24	9	S	26	0.330		
25	10	S	24	0.453		
26	11	K	24 spiked	0.301		
27	907	QC1	CRM (0.8mg/L)	0.242		
28	0	B	Baseline	0.000		
29	921	D	Drift	2.401		
30	12	S	28	0.227		
31	13	S	30	0.247		
32	14	S	38	0.342		
33	15	S	39	0.322		
34	16	S	40	0.445		
35	17	S	41	0.400		
36	18	S	42	0.450		
37	19	S	43	0.395		
38	20	S	44	0.415		
39	21	S	45	0.396		
40	22	K	45 spiked	0.237		
41	907	QC1	CRM (0.8mg/L)	0.251		
42	0	B	Baseline	0.000		

43	921	D	Drift	2.401
44	23	S	46	0.383
45	24	S	47	0.280
46	25	S	48	0.308
47	26	S	50	0.076
48	27	S	51	0.295
49	28	S	52	0.304
50	29	S	53	0.281
51	30	S	54	0.253
52	31	S	55	0.241
53	32	S	49	0.319
54	33	K	49 spiked	0.368
55	907	QC1	CRM (0.8mg/L)	0.253
56	0	B	Baseline	0.000
57	921	D	Drift	2.401
58	34	S	56	0.264
59	35	S	57	0.275
60	36	S	58	0.280
61	37	S	59	0.274
62	38	S	60	0.241
63	39	S	61	0.316
64	40	S	62	0.309
65	41	S	63	0.283
66	42	S	64	0.273
67	43	S	65	0.309
68	44	K	65 spiked	5.317 *
69	907	QC1	CRM (0.8mg/L)	0.252
70	0	B	Baseline	0.000
71	921	D	Drift	2.401
72	45	S	67	0.304
73	46	S	68	0.349
74	47	S	70	0.257
75	48	S	71	0.247
76	49	S	72	0.330
77	50	S	73	0.254
78	51	S	74	0.265
79	52	K	74 spiked	0.276
80	907	QC1	CRM (0.8mg/L)	0.214
81	0	B	Baseline	0.000
82	921	D	Drift	2.401
83	0	B	Final Base	0.000

Corrections

Channel	3
Baseline	done
Drift	done
Carryover	done
%	0.10

Spike Recovery


Blank spiked Added	0.075
Blank spiked Found	0.024
Recovery %	31.953
24 spiked Added	0.055
24 spiked Found	-0.152
Recovery %	-274.600
45 spiked Added	0.060
45 spiked Found	-0.159
Recovery %	-264.105
49 spiked Added	0.067
49 spiked Found	0.049
Recovery %	73.098
65 spiked Added	0.067
65 spiked Found	5.008
Recovery %	7421.148
74 spiked Added	0.071
74 spiked Found	0.011
Recovery %	16.101

Calibration

Channel 3 TKN

Type	Observed	Calculated	Target	% Error
1C	58681	2.379	2.240	6.23
2C	45336	1.798	1.680	6.99
3C	31741	1.205	1.120	7.56
4C	18259	0.617	0.560	10.13
5C	9938	0.254	0.224	13.34
6C	9488	0.234	0.000	-

Calibration Fit: Slope only
 Correlation Coefficient: 0.9966
 Carryover (%): 0.1033
 Calibration Equation: $y = bx$
 y = Peak Height Digit. Units
 x = Concentration Unit mg/L
 a = 0.000000E+000
 b = 2.293176E+004

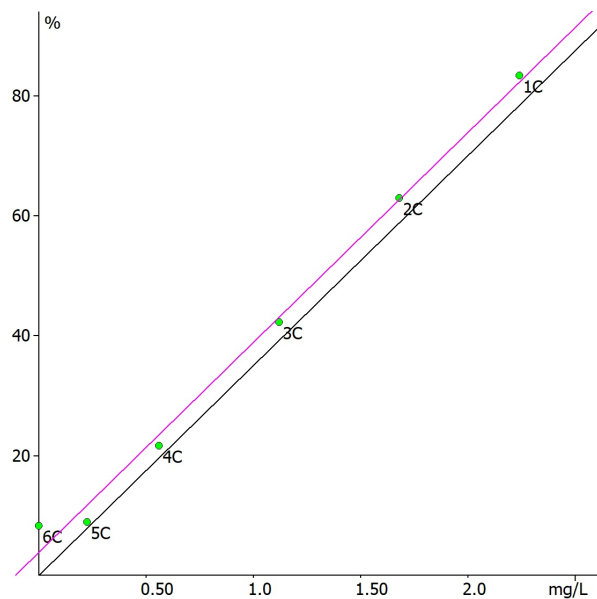

Legend

* ... Sample offscale
 + ... Result higher than sample limit
 - ... Result lower than sample limit
 P ... Standard passed
 F ... Standard failed
 N ... Value not calculated or not used
 R ... Resample after offscale
 M ... Peak marker moved manually
 d ... Pre-Diluted sample
 D ... Post-Diluted sample
 H ... Dual calibration used
 Z ... Report negative values as zero