

General

Name of Run	241212_NP1_Sample321.run	Name of Analysis	NOx_P04.ANL
Date of Report	12/12/2024	System	AA500
Run Start	12/12/2024 4:09:20 PM	Run Stop	4:30:34 PM
Operator Run/Rec.	CLMR	Software Version	AACE 8.02 SP2
Comment	Sample appeared "soapy" Sample had a different viscosity/"soapy" 241212_Q7_NP1.run		

Parameters

Channel	1	3	
Method	NOx	P04	Dilution
Unit	mg/L	mg/L	
Calib. Fit	Linear	Linear	
Corr.Coeff.(r)	0.9999	0.9999	
AUFS/Gain	0.45/22	0.10/101	Data
Offset	158	4879	Field
Sensitivity	0.3648	0.0833	'#2
Sample Limit 1	-	-	
Sample Limit 2	-	-	

Results

Pk	Cup	Type	Sample ID	Value	Value	Data
0	0	B	Initial Base	-0.003	-0.006	0
1	921	P	Primer	0.196	0.198	1
2	921	D	Drift	0.198	0.199	1
3	910	S	321	0.004	0.000	1
4	906	S	Blank	-0.001	0.000	1
5	908	QC1	CRM 7/15 [0.15/0.03]	0.148	0.023	1
6	909	QC1	CRM 4/30 [0.15/0.03]	0.148	0.026	1
7	0	B	Baseline	-0.003	-0.006	1
8	921	D	Drift	0.198	0.199	1
9	0	B	Final Base	-0.003	-0.006	1

Corrections


Channel	1	3
Baseline	done	done
Drift	done	done
Carryover	none	none
%	0.00	0.00

Calibration

Channel 1 NOx

Type	Observed	Calculated	Target	% Error
1C	57131	0.200	0.200	0.08
2C	30420	0.099	0.100	-0.62
3C	17382	0.050	0.050	0.37
4C	10928	0.026	0.025	3.33
5C	6604	0.010	0.010	-4.83
6C	5723	0.006	0.005	23.87
7C	3748	-0.001	0.000	-


Calibration Fit: Linear
 Correlation Coefficient: 0.9999
 Carryover (%): 0.0000
 Calibration Equation: $y = bx + a$
 y = Peak Height Digit. Units
 x = Concentration Unit mg/L
 a = 4.081494E+003
 b = 2.650398E+005

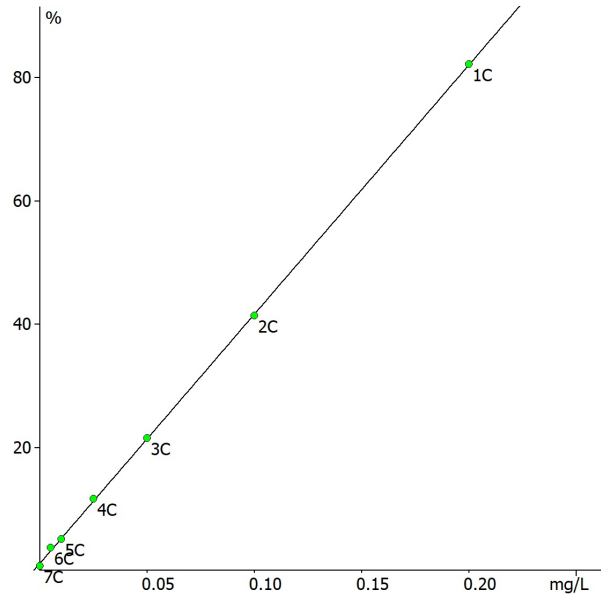

Channel 3 P04

Type	Observed	Calculated	Target	% Error
1C	58650	0.199	0.200	-0.40
2C	32109	0.101	0.100	1.29
3C	18441	0.051	0.050	1.72
4C	11261	0.024	0.025	-2.52
5C	7447	0.010	0.010	2.99
6C	5985	0.005	0.005	-1.89
7C	4403	-0.001	0.000	-

Calibration Fit: Linear
 Correlation Coefficient: 0.9999
 Carryover (%): 0.0000
 Calibration Equation: $y = bx + a$
 y = Peak Height Digit. Units
 x = Concentration Unit mg/L
 a = 4.655349E+003
 b = 2.710476E+005

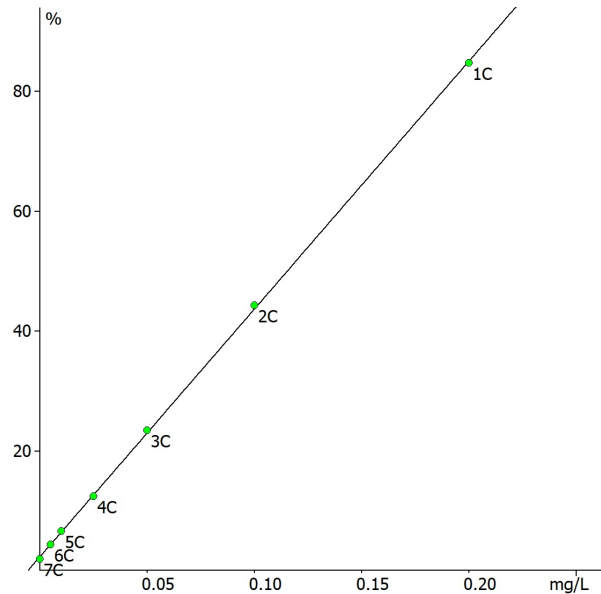

Legend

* ... Sample offscale
 + ... Result higher than sample limit
 - ... Result lower than sample limit
 P ... Standard passed
 F ... Standard failed
 N ... Value not calculated or not used
 R ... Resample after offscale
 M ... Peak marker moved manually
 d ... Pre-Diluted sample
 D ... Post-Diluted sample
 H ... Dual calibration used
 Z ... Report negative values as zero