


(1) Combination of slice selection gradient and RF pulse excites one slice only

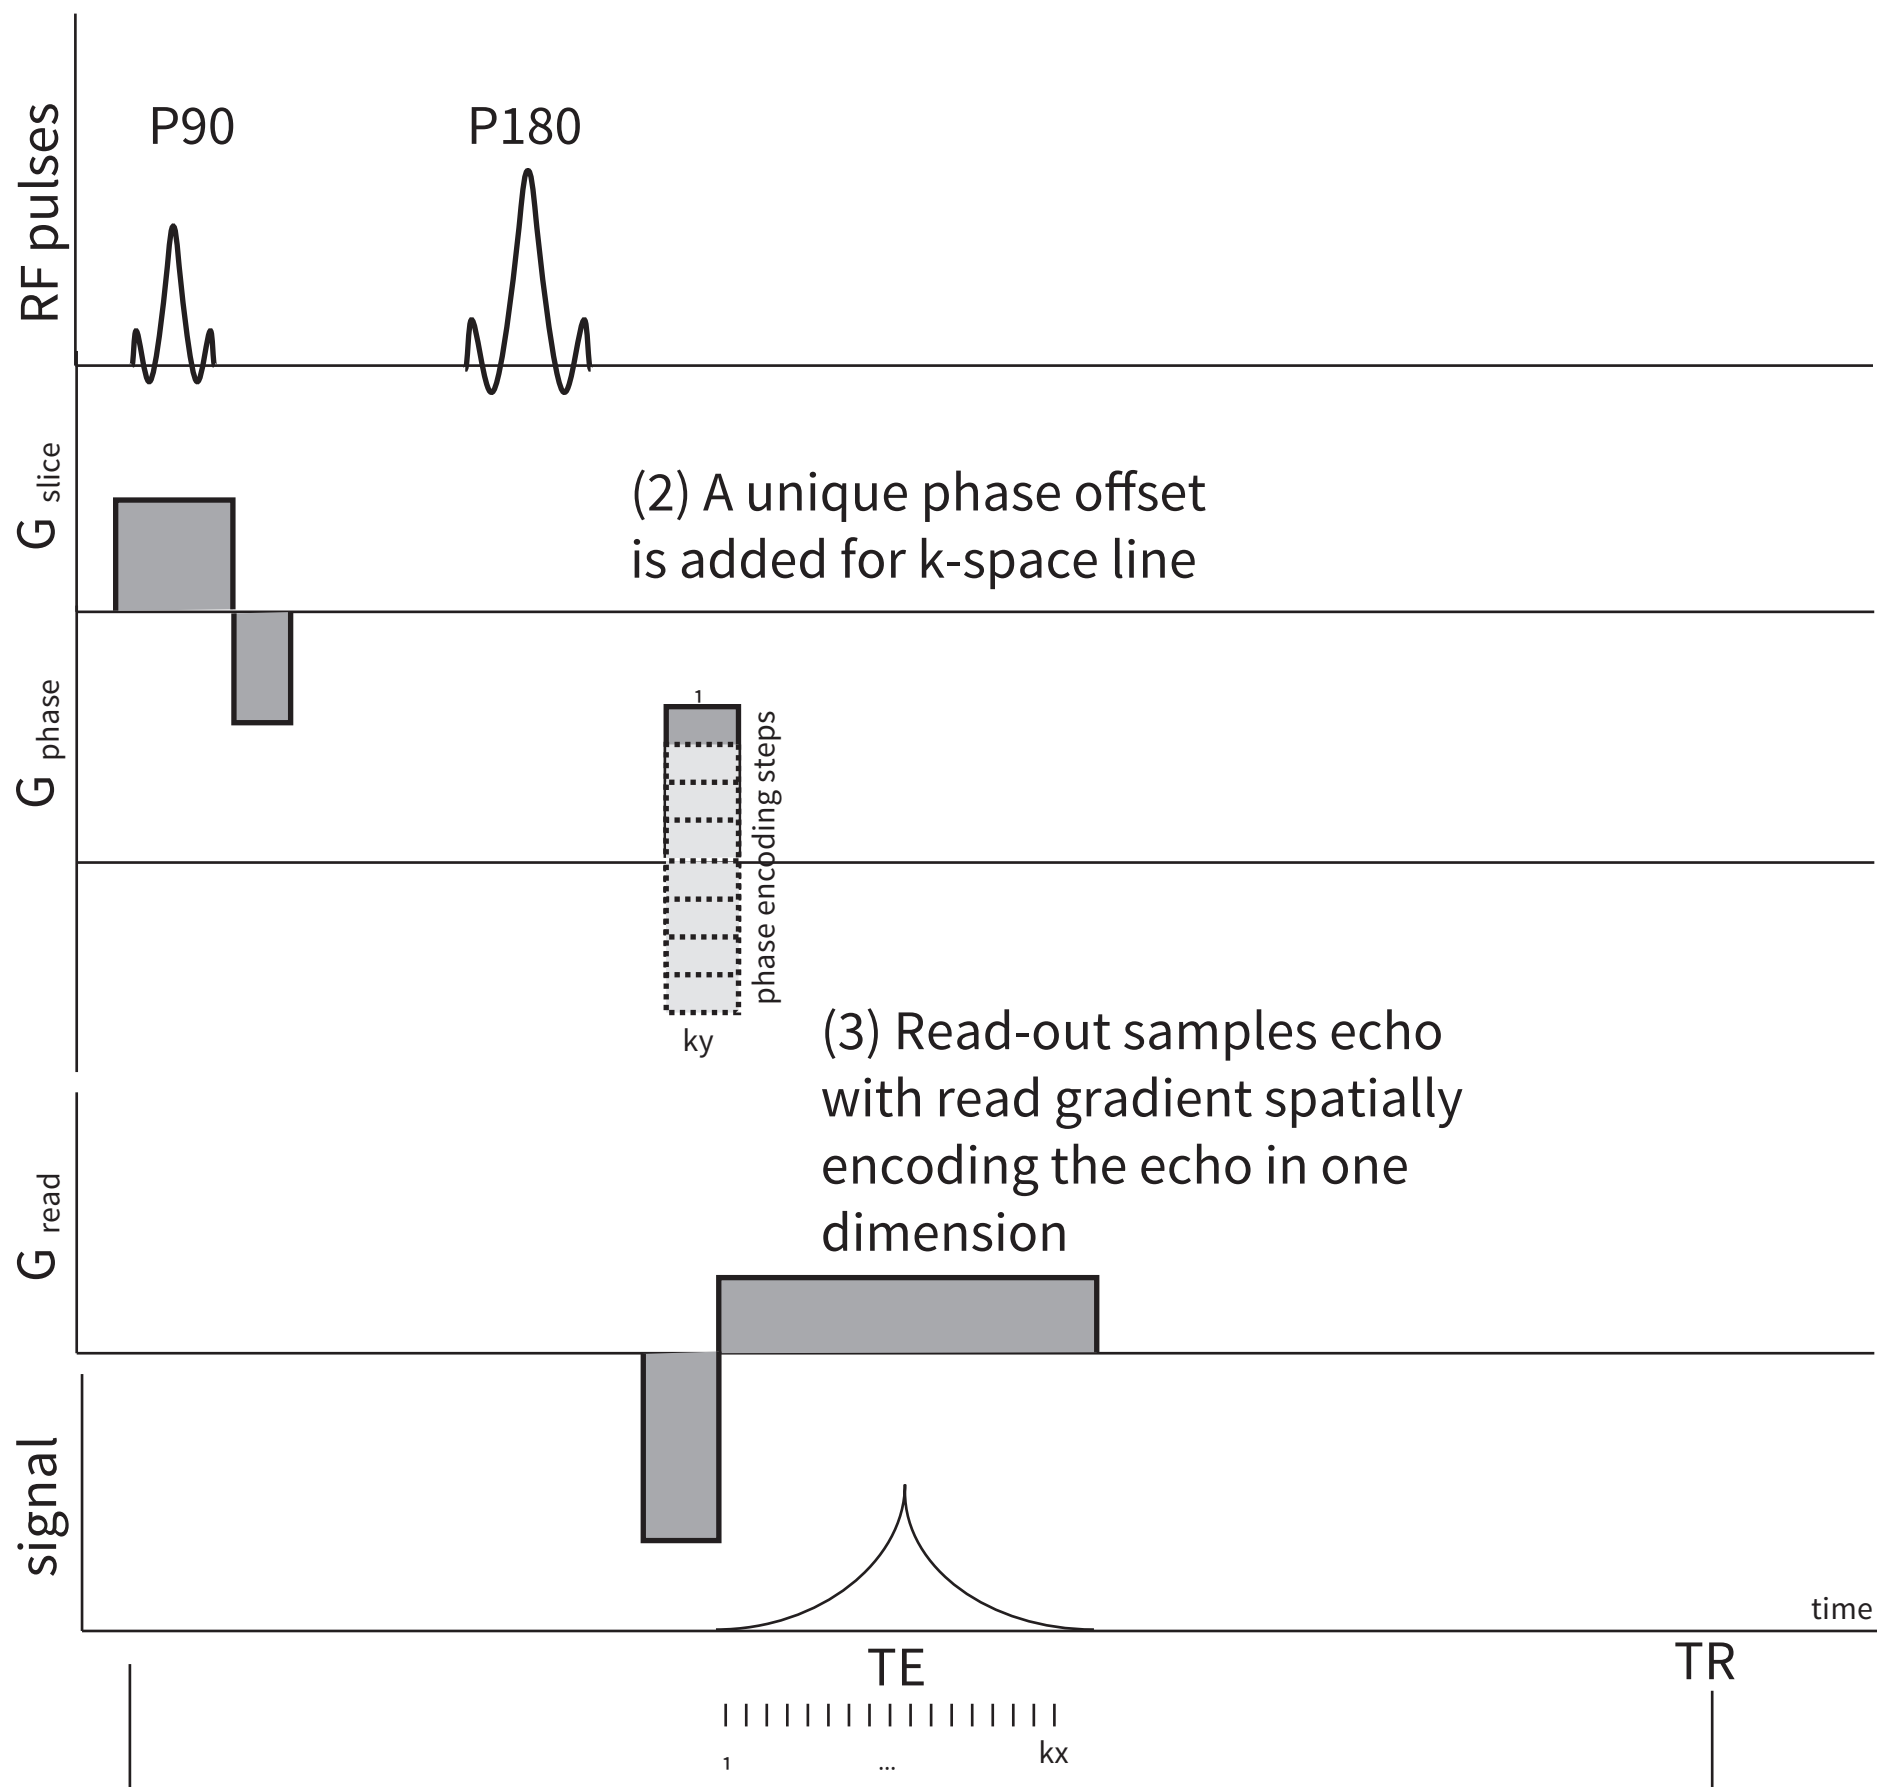

(2) A unique phase offset is added for k-space line

(3) Read-out samples echo with read gradient spatially encoding the echo in one dimension

(4) repeat for each line in k-space