


## Wellness journey vital signs

We have three different places where we collect vitals (heart rate, blood pressure, etc.) One is on the phase one slide out, another is on the phase 2 event logging of timestamps And one is on the phase 2 Control panel. We need to decide where we want that and should probably just have one.

The screenshot shows a mobile application interface titled "SESSION UPDATE". At the top, it displays the time "T+00:01:29 - 12:01:57 AM". Below this, there are two dropdown menus: "PATIENT AFFECT" set to "Calm" and "RESPONSIVENESS" set to "Fully responsive". There are also input fields for "HR (BPM) - OPTIONAL" (e.g. 88) and "SYSTOLIC - OPTIONAL" (e.g. 120). A text input field for "SESSION NOTE - OPTIONAL" contains the placeholder "Brief observation (no PHI) ...". At the bottom, a note states "Session-local only – exported with session summary. Not logged to the database." A large green button at the bottom is partially visible.


## Substance Library

"2 Documented interactions" Leads to Dashboard

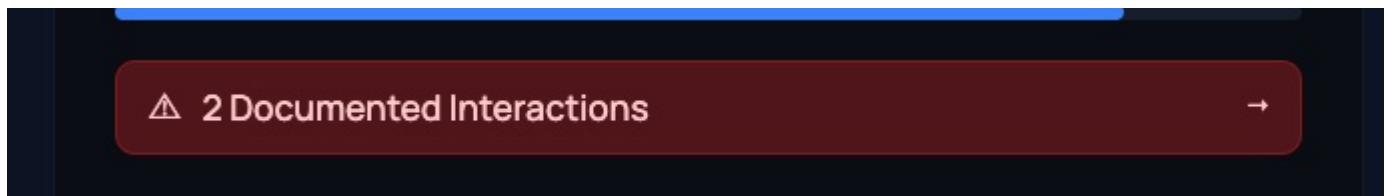


## Substance Monograph

Substance filter opens up, off the page; should open down

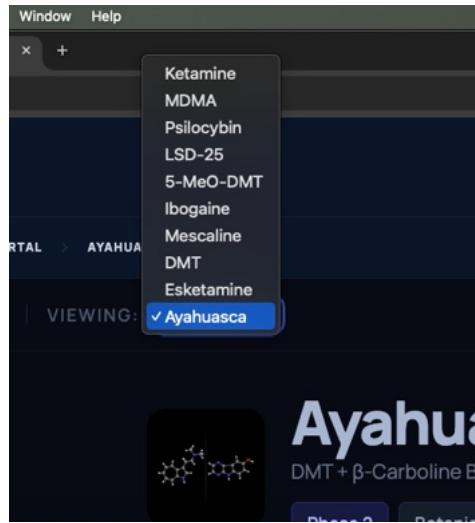

## Monograph

Spider graph highlights with a box around it and cursor will not select; hover selection only

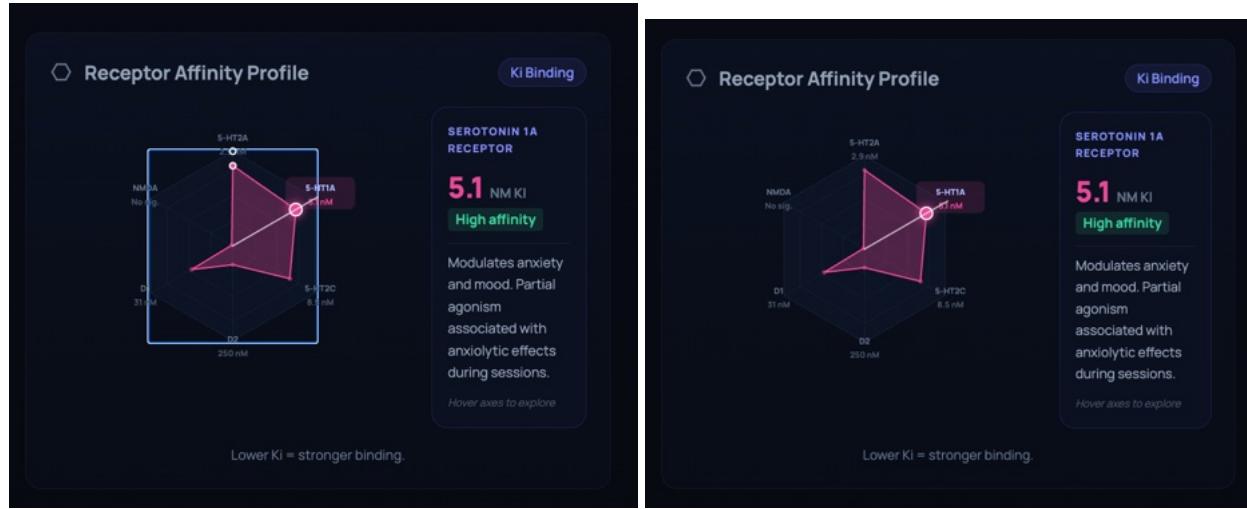

## Sidebar

Mobile Scanner and Device Sync lead to the same modal; neither has instructions

Connect your mobile device to scan documents directly into the patient record.

## 📱 Mobile Scanner ⊕

Instantly beam this session to your mobile device or wearable for remote monitoring.

## ⌚ Device Sync ⊕



Scan with camera

### Send to Phone

The Mobile Scanner tool is specifically optimized for a mobile-first interface. Scanning this secure code will instantly beam your current session context to your device.

- 1 Open your smartphone's native camera app.
- 2 Point the camera directly at the QR code.
- 3 Tap the PPN link that appears to instantly authenticate.

**ZERO-FRICTION HANDOFF**  
No app store download. No typing passwords.  
Instantly securely bonded.



Scan with camera

### Send to Phone

The Device Sync tool is specifically optimized for a mobile-first interface. Scanning this secure code will instantly beam your current session context to your device.

- 1 Open your smartphone's native camera app.
- 2 Point the camera directly at the QR code.
- 3 Tap the PPN link that appears to instantly authenticate.

**ZERO-FRICTION HANDOFF**  
No app store download. No typing passwords.  
Instantly securely bonded.



### Send to Phone

The Device Sync tool is specifically optimized for a mobile-first interface. Scanning this secure code will instantly beam your current session context to your device.

- 1 Open your smartphone's native camera app.
- 2 Point the camera directly at the QR code.
- 3 Tap the PPN link that appears to instantly authenticate.



**ZERO-FRICTION HANDOFF**  
No app store download. No typing passwords.  
Instantly securely bonded.

## Clinic Performance radar

Has scroll bar inside component missing filters


## Clinic Performance Radar

This dashboard tracks how well a clinic is improved patient outcomes. It measures key performance indicators like remission rates and patient retention to help optimize care.

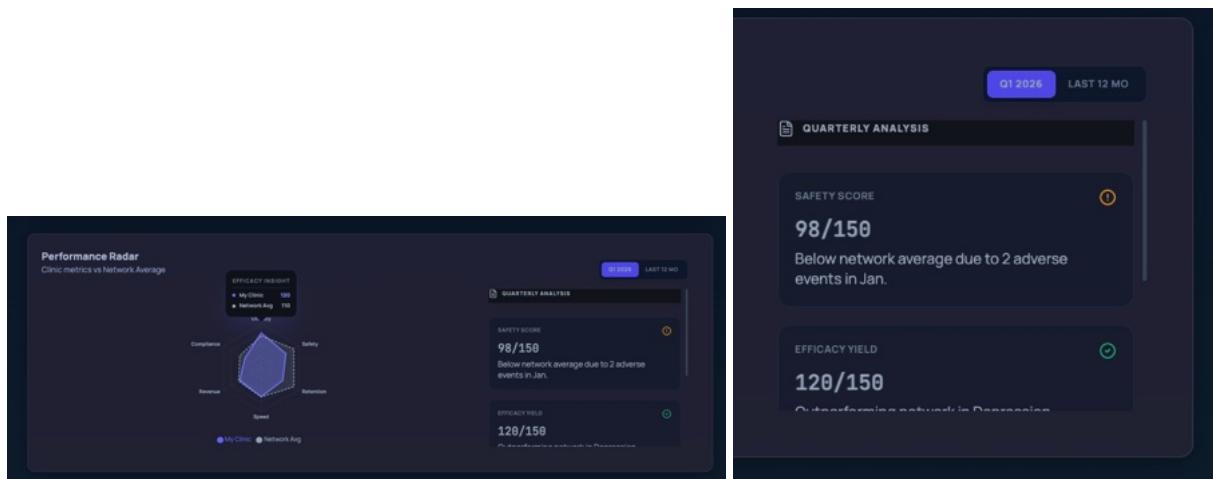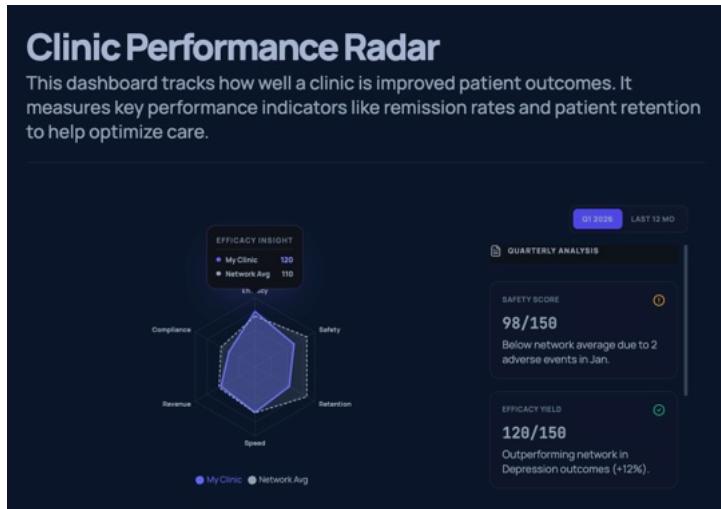


## Safety Surveillance Matrix

This is a great page and needs to be available on the site; it's not currently displayed anywhere. check filters and data connection

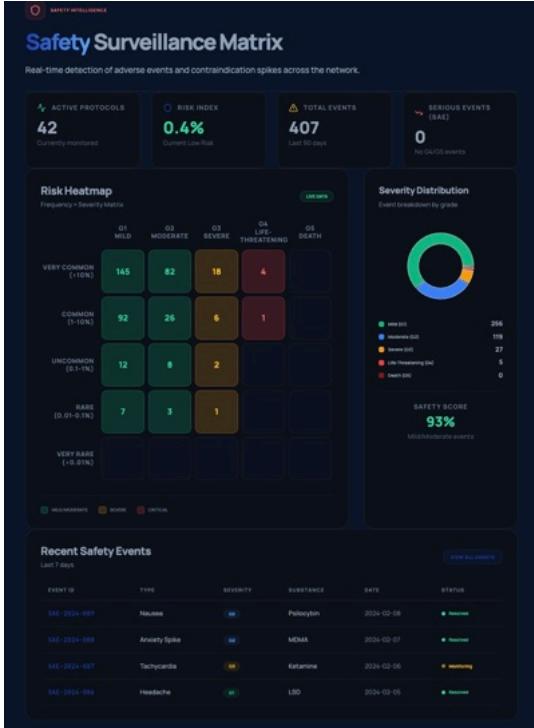


## Wellness Journey Phase 2 Companion

Everyone loves this feature. Video disappeared; Video needs to be inside a full page container so it sizes dynamically and doesn't get covered by the buttons

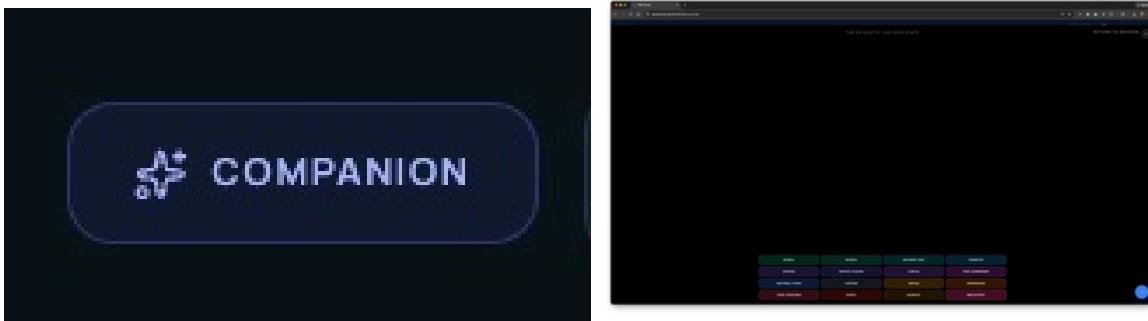

## Progressive web app modal

Opens at the very top of the screen; cut off; can't escape or exit out

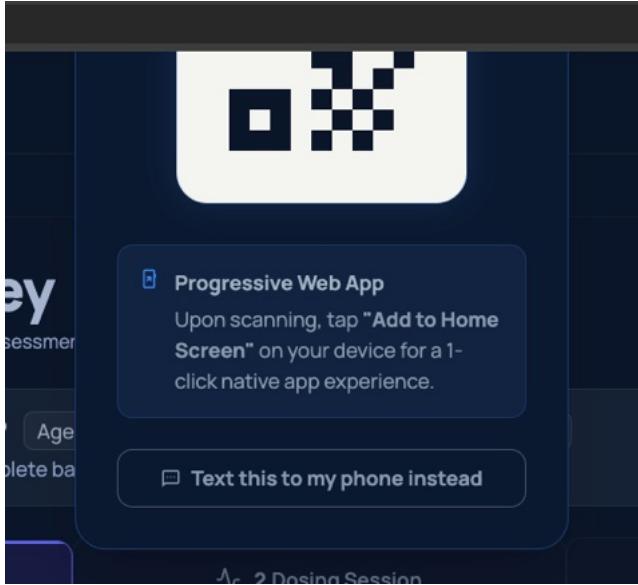



## Wellness Journey Phase 1

Initial modals are not escaping properly

Report tooltips are automatically opening and cut off to the right by the container; should be optional and open inward toward the center

A few AIL Right-corner tooltips cut off inside their container site-wide

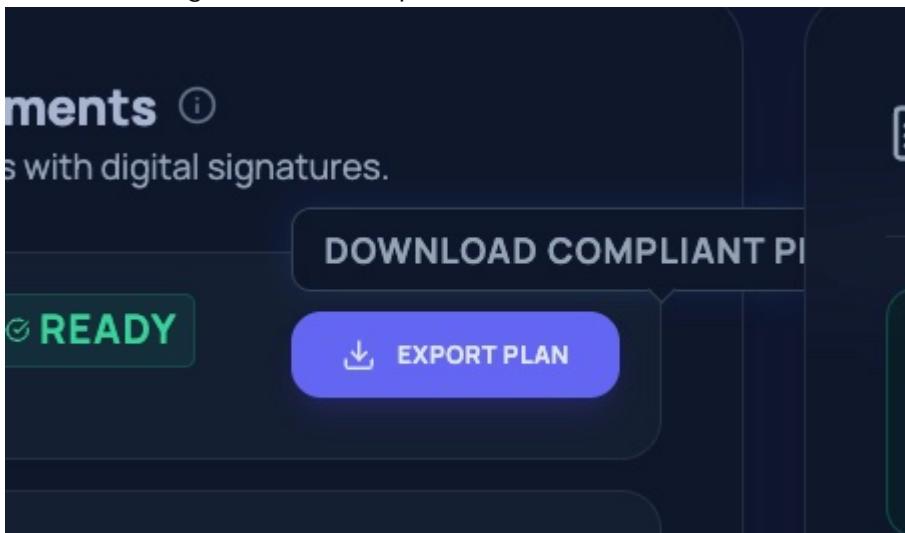

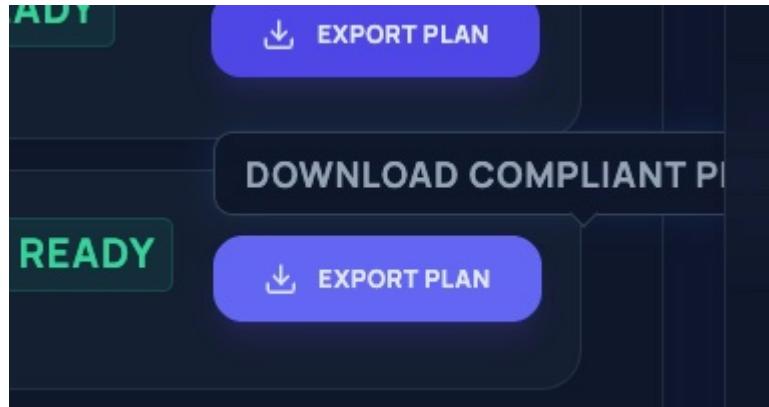

Wellness journey guided tours don't move, but pressing the tab button moves around the blurred screen behind the modal