


Pareto Chart for Non-Fatal Pacemaker Failures

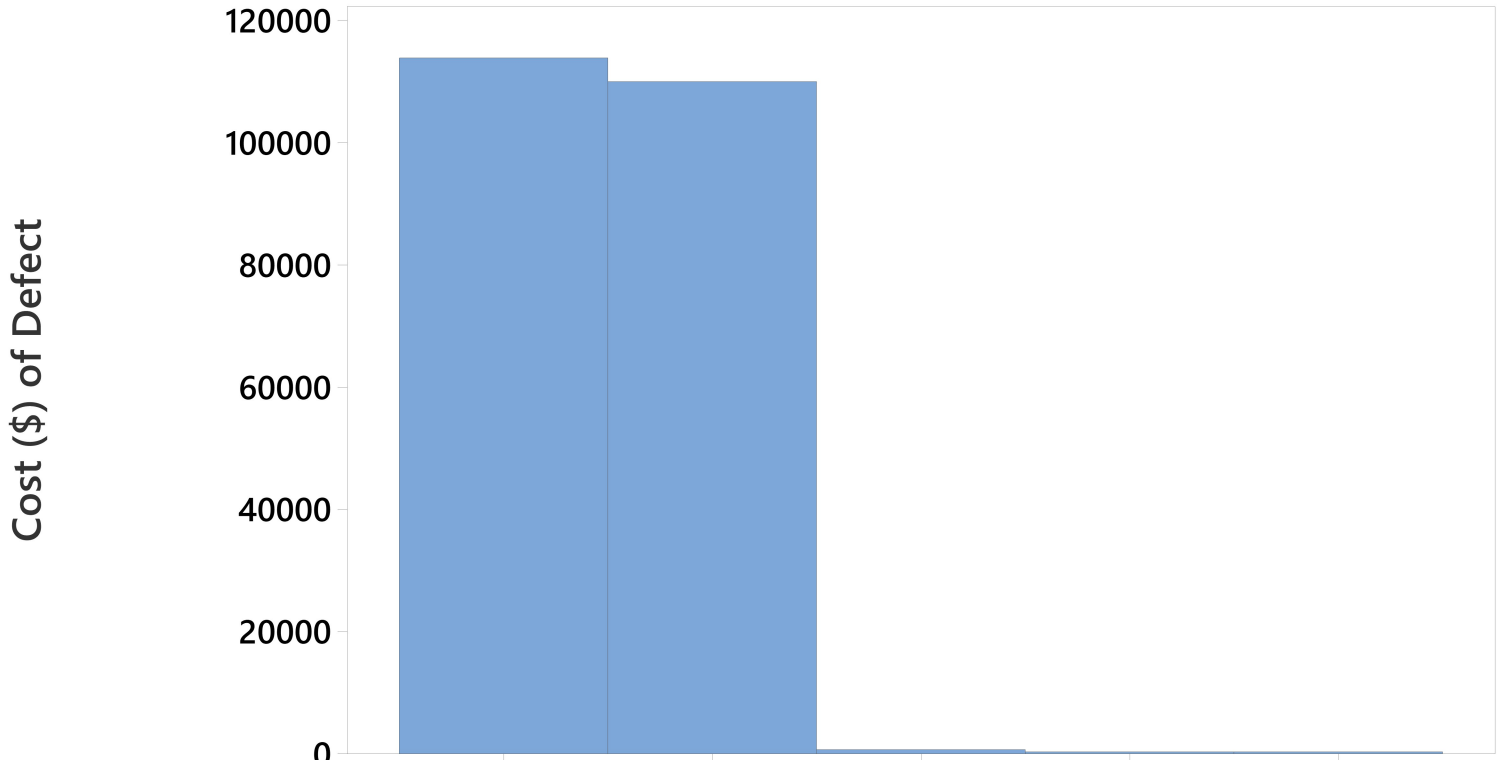

Type of Defect	Battery Life	Electro Shielding	Irreg. Heart Beat	Discomfort	Lethargy
Cost (\$) of Defect	113850	110000	700	350	350
Percent	50.5	48.8	0.3	0.2	0.2
Cum %	50.5	99.4	99.7	99.8	100.0