Loan Container Incoming Inspection

icotec Cervical Cage

Overview Instrumentation

- **Configuration of the container (41-12):**
  - Inserter sleeve 41-13-1 or 41-13-3
  - Inserter rod 41-13-2
  - Inserter sleeve, long 41-13-4
  - Inserter rod, long 41-13-5

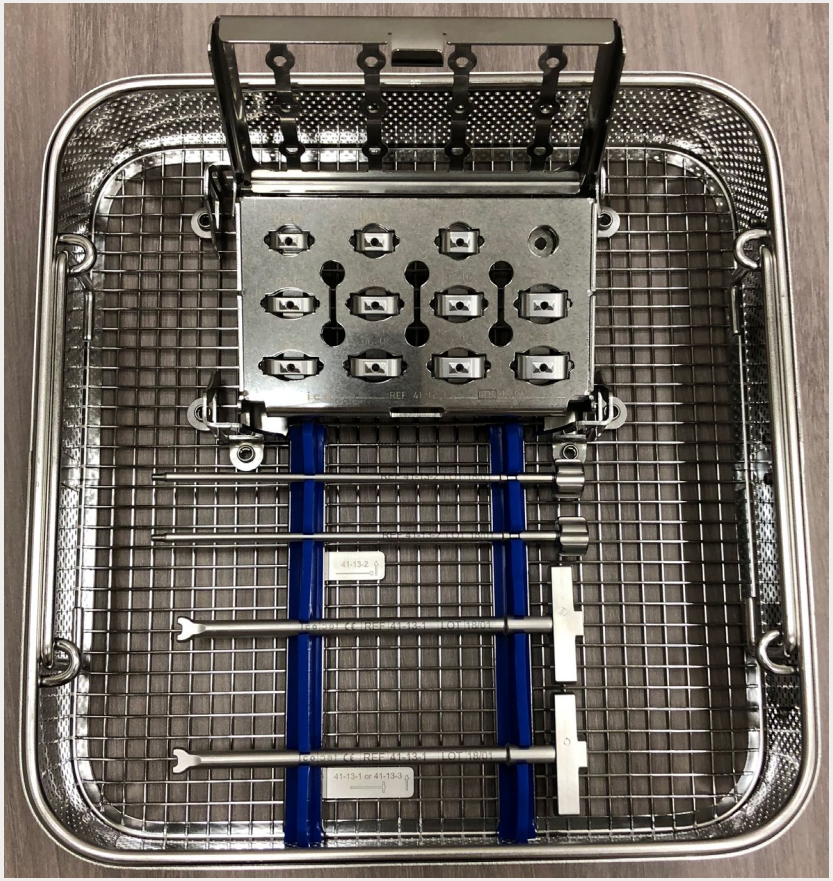

General Control

- **Do the contents of the container correspond to the kit profile?**
- **Are the instruments intact (not clearly damaged)?**
- **Is the laser marking legible/the data matrix code visible?**
  - Instruments where the laser marking is no longer legible must be replaced.
  - Instruments where the data matrix code (UDI) is no longer visible must be replaced. (When available, a scanner can be used to check the data matrix code.)

- **Movable parts/joints – maintenance using surgical instrument oil!**

  → **Functional inspections for instruments** (see following pages)

- **If an instrument is replaced, all tests involving this instrument have to be repeated.**
- **Instructions for Reprocessing: 0126US**

Functional Inspection

- **Inserter Sleeve without or with Depth Limiter (41-13-1 or 41-13-3) or Inserter Sleeve, long (41-13-4) and Inserter Rod (41-13-2) or Inserter Rod, long (41-13-5)**
  - Insert the inserter rod in the inserter sleeve
  - The thread must project out (marked in red)
  - The inserter rod must not fall out due to its own weight
  - The inserter rod can be turned with just minimal friction

- **Cervical Insertion Instrument MIS and Probe**
  - All probes can be mounted securely on the insertion instrument and do not wobble

0181US.2025-06