Loan Container Incoming Inspection

icotec Anterior Cervical Plate

confidential, property of icotec ag, Switzerland

Overview Instrumentation

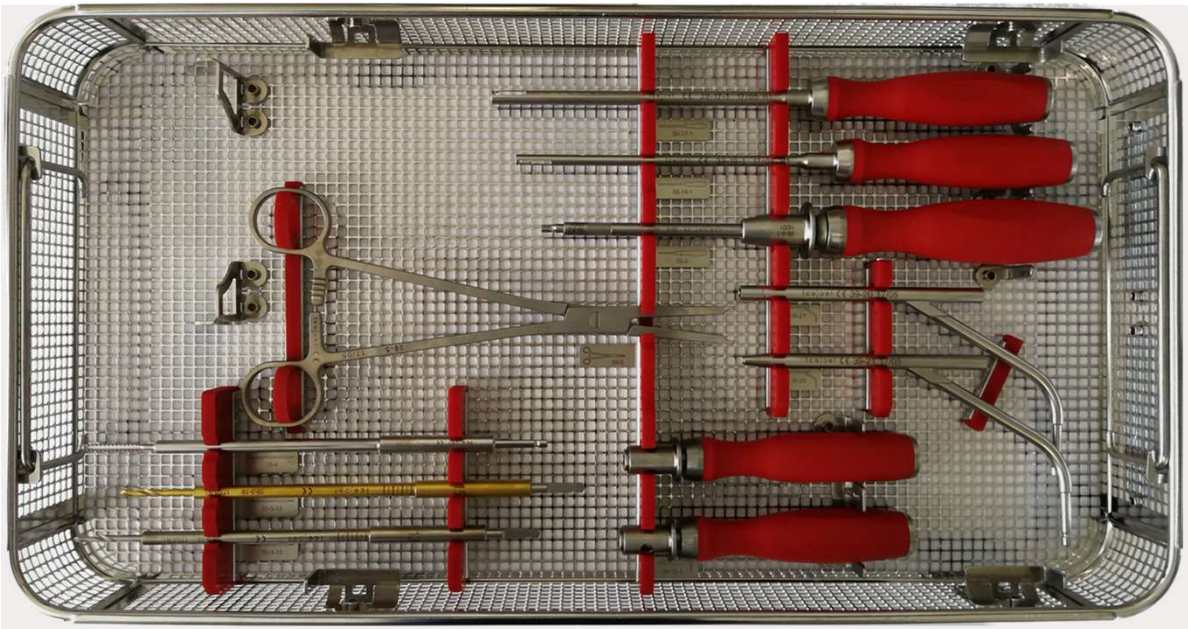

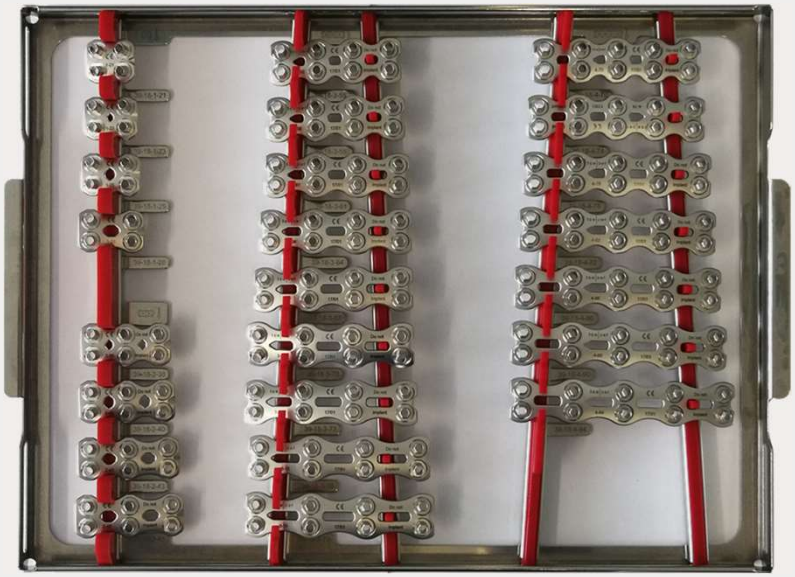

or

Overview Inspection Aids

Screw Ø 4.0 × 13 mm (H279)

General Control

- **Do the contents of the container correspond to the kit profile?**
- **Are the instruments intact (not clearly damaged)?**
- **Is the laser marking legible/the data matrix code visible?**
  - Instruments where the laser marking is no longer legible must be replaced.
  - Instruments where the data matrix code (UDI) is no longer visible must be replaced. (When available, a scanner can be used to check the data matrix code.)

- **Movable parts/joints – maintenance using surgical instrument oil!**

  → **Functional inspections for instruments** (see following pages)

- **If an instrument is replaced, all tests involving this instrument have to be repeated.**
- **Instructions for Reprocessing: 0061US**

Functional Inspection

- **Fixation Pin (39-17-3) and Template/Fixation Pin Holder (39-17-1)**
  - Should move easily, fixation pin must not fall off due to its own weight

- **Mini Drill Sleeve (39-17-2) and Template/Fixation Pin Holder (39-17-1)**
  - Should move easily, mini drill sleeve must not fall off due to its own weight

Functional Inspection

- **Template (39-18-X-XX) and Template/Fixation Pin Holder (39-17-1)**
  - Should move easily, template must be removable without much effort
  - Test on 1 entire template

- **Positioning Pin for Template (39-19-2) and Positioning Pin Driver (39-19-1)**
  - Should move easily, but positioning pin for template must not fall out

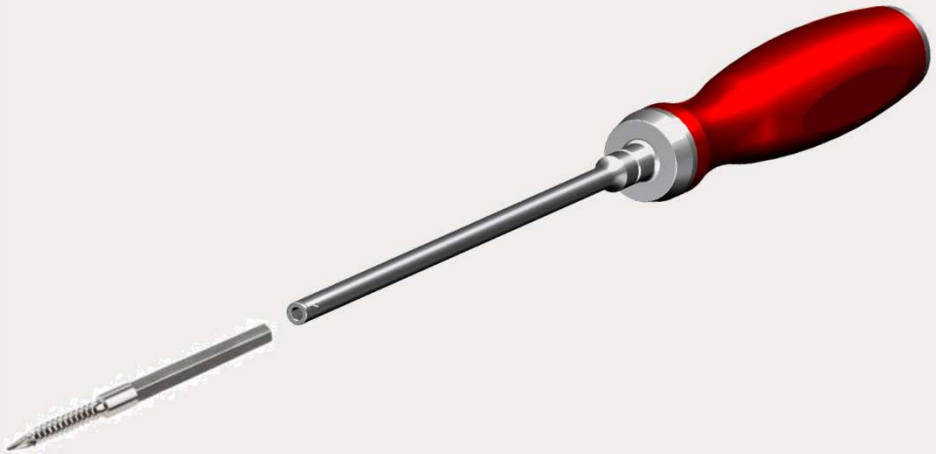

Functional Inspection

- **Screwdriver (39-8)**
  - Is the tip intact?
  - Blade can be pushed smoothly over the sleeve with low friction
  - Can the screwdriver be disassembled and reassembled?
  - Dimensional check of the tip with a screw
    - Can the screw Ø 4.0 × 13 mm (H279) be mounted onto the screwdriver by pulling back the sleeve? Sleeve has to be released after picking up the screw
    - The screw must not wobble on the screwdriver (shake test)
  - Movable parts/joints – maintenance using instrument oil!

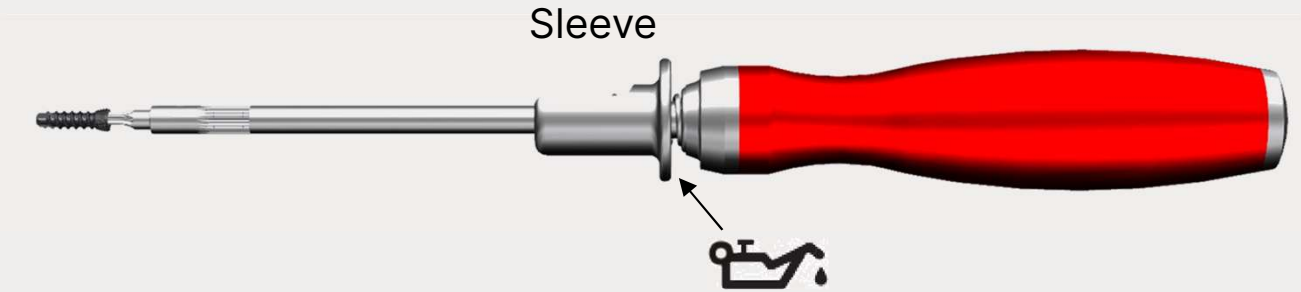

Functional Inspection

- **Drill (39-3-13, 39-3-15) and Drill Sleeve for Template (39-20)**
  - Should move easily, does not get caught
  - Do the drills reach the depth stop of the drill sleeves?

- **Forceps for Implant (39-5)**
  - Can be moved and engaged with low friction
  - Movable parts/joints – maintenance using surgical instrument oil!

Functional Inspection

- **Drill (39-3-13, 39-3-15) and Conical Drill Sleeve for Plate (39-21)**
  - Should move easily, does not get caught
  - Do the drills reach the depth stop of the drill sleeves?

- **Drill (39-3-13, 39-3-15) and Tap (39-4)**
  - Concentricity check (roll on edge of table)
  - Gold-colored coating on drills intact?
  - Black marker lines visible?
  - Drill tip still sharp-edged? Is the drill twisted evenly?

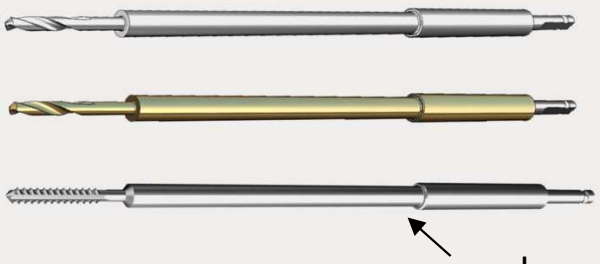

Functional Inspection

- **Drill Sleeve for Template (39-20) with Template (39-18-X-XX)**
  - Can be mounted with minimal effort
  - Template must be easy to remove from drill sleeve, no self-holding mechanism
  - Test on 1 entire template

- **Grip, AO Coupling (39-15-1)**
  - 2 drills and 1 tap can be engaged with AO coupling
  - 2 drill sleeves can be engaged with AO coupling
  - Movable parts/joints – maintenance using surgical instrument oil!

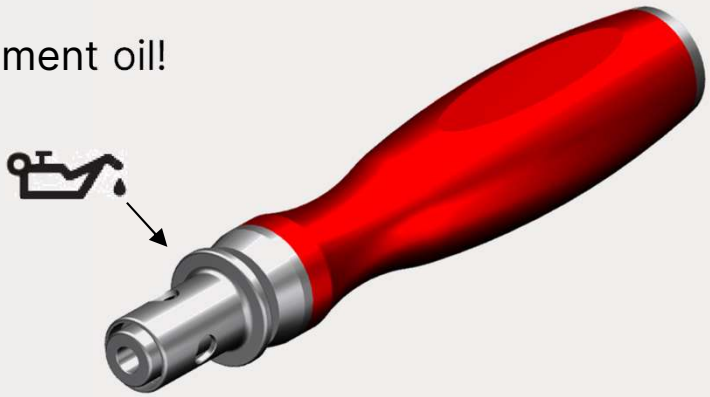

0196US.2025-06