

A

Hour 0

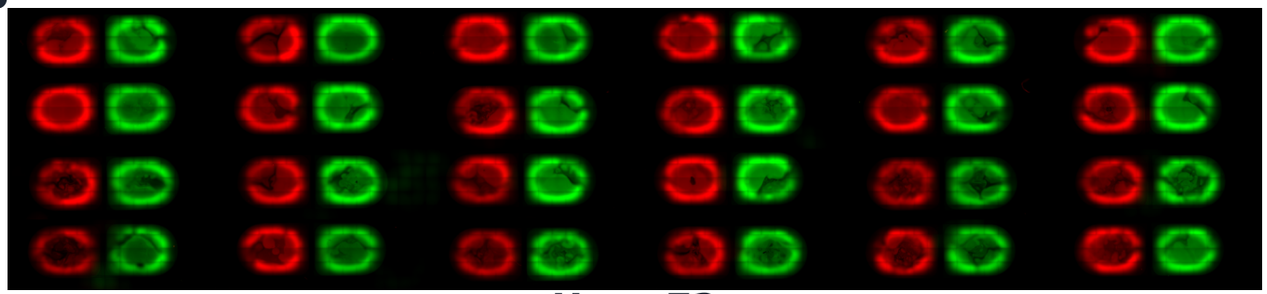


Hour 72

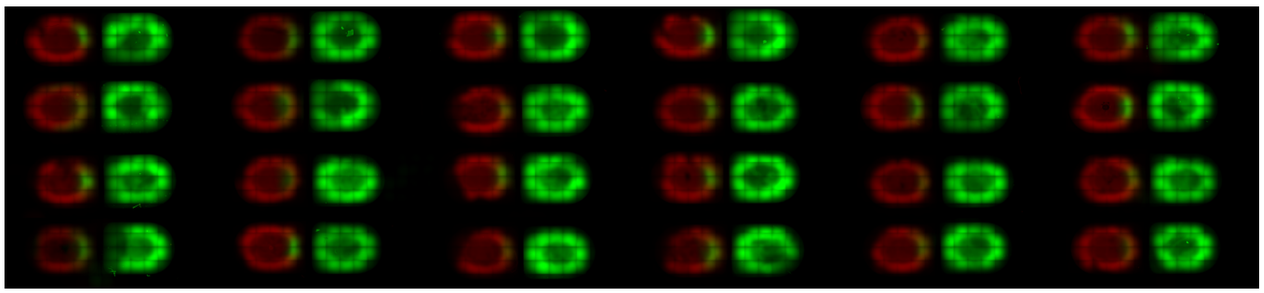


B

CTβ-647 labeling at DIV11

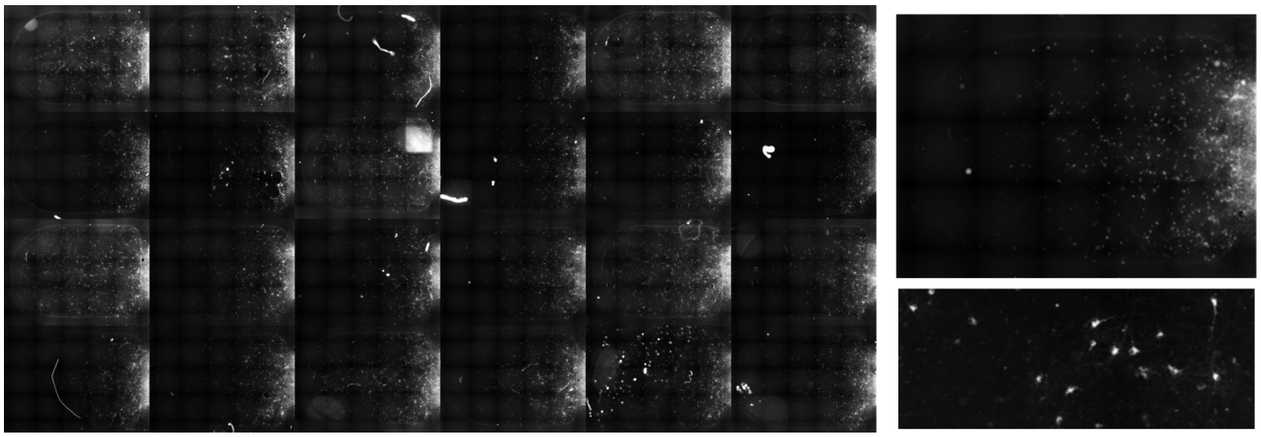

C

Mean CTβ-positive cell-body count per analyzed device

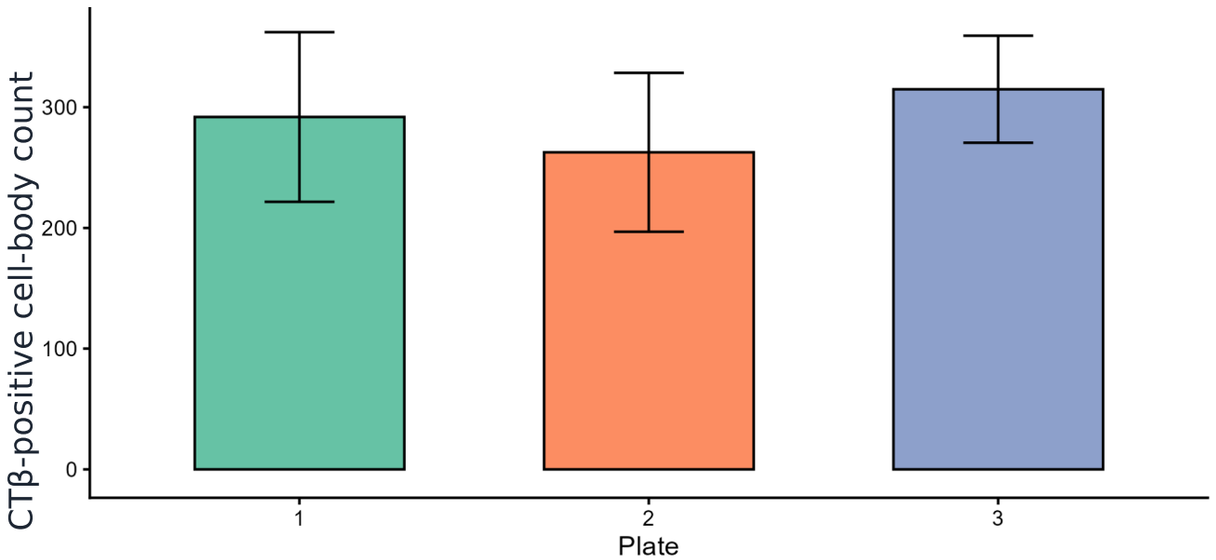

Bars: plate mean; error bars: SD across analyzed interior devices
Neurons from one E18 rat embryo; three plates; 69 devices analyzed