

Photoreceptor mechanisms underlying physiological responses to bright light in humans

Lucien Bickerstaff^{1, 2} [\[0000-0002-2683-8130\]](#) *, Josef Trinkl¹ [\[0009-0008-9064-4972\]](#), Stephan Munkwitz¹ [\[0000-0002-9559-5566\]](#), Johannes Zauner² [\[0000-0003-2171-4566\]](#) & Manuel Spitschan^{1, 2, 3, 4} [\[0000-0002-8572-9268\]](#) *

¹ Max Planck Institute for Biological Cybernetics, Translational Sensory & Circadian Neuroscience, Tübingen, Germany

² Technical University of Munich, Chronobiology & Health, TUM School of Medicine and Health, Munich, Germany

³ Technical University of Munich, TUM Institute for Advanced Study (TUM-IAS), Garching, Germany

⁴ TUMCREATE, Singapore, Singapore

* Corresponding authors: Manuel Spitschan (manuel.spitschan@tum.de), Lucien Bickerstaff (lucien.bickerstaff@tuebingen.mpg.de)

Abstract

Ocular light can produce responses in the human body that are not mediated by the fundamental and more well-known functions of the human visual system, and that often involve complex and not well-understood interactions within the nervous system. Sensitivity to light shows sizeable variability between individuals, and the underlying photoreceptor mechanisms remain partially unclear. To fill in this knowledge gap, this study operationalises acute light sensitivity responses, using objective (facial surface electromyography [sEMG], pupillometry) as well as subjective (scale-measured self-reporting) approaches in healthy adults ($n = 20$, age range 18-35). Within each of the four sessions, 36 successive light pulses from six narrowband wavelengths are delivered through a spectrally tuneable LED based light engine (445, 465, 475, 505, 525, 545 nm) under homogenous, full field stimulation at a fixed irradiance. We hypothesise that predicting visual discomfort using melanopic EDI (tuned to ipRGCs) will provide a better fit compared to using illuminance (tuned to L+M cones).

33 Abbreviations

34

ACHOO	Autosomal Dominant Compelling Helioophthalmic Outburst
AIC	Akaike's Information Criterion
AUDIT	Alcohol Use Disorders Identification Test
BAC	Blood Alcohol Content
DC	Direct Current
EDI	Equivalent Daylight Illuminance
HRR	Hardy Rand and Rittler
ipRGC	Intrinsically Photosensitive Retinal Ganglion Cell
IR	Infrared
KSS	Karolinska Sleepiness Scale
LED	Light Emitting Diode
LLM	Large Language Model
LMM	Linear Mixed Model
OD	Optical Density
PCA	Principal Component Analysis
PLR	Pupillary Light Reflex
RGB	Red, Green, Blue
RHT	Retinohypothalamic Tract
SCN	Suprachiasmatic Nucleus
sEMG	Surface Electromyography
SPD	Spectral Power Distribution

35

Introduction

It is well known that light is essential for many physiological functions of the human body, regulating many visual as well as non-visual processes. The latter include notably pupil size regulation, cognitive and affective processes, and circadian entrainment – all mediated by the melanopsin-containing, intrinsically photosensitive retinal ganglion cells (ipRGCs)^{1,2}. These cells affect circadian rhythms through projection to the suprachiasmatic nucleus (SCN) via the retinohypothalamic tract (RHT) but also have projections to other brain areas which directly drive behaviour and cognitive function^{2,3}. Responding to bright light exposure is a phenomenon that many humans will be familiar with. These responses occur under a broad range of lighting conditions and typically translate into a characteristic set of physiological responses, e.g. eye closure, pupil constriction, facial muscle contraction, and/or other light-avoiding behaviours.

Visual functions are regulated by well-known photoreceptors, namely cones and rods. These lie at the back of the retina, which is a fine layer of nerve tissue. Cones allow for colour vision, spatial detail and motion perception during daytime. They are most dense in the fovea (centre of the retina), and exist in three subtypes differing in the opsins they contain, each sensitive to varying wavelengths of light – conveniently named L (long-wavelength-sensitive, peaking at ~565 nm), M (medium-wavelength-sensitive, peaking at ~535 nm), and S (short-wavelength-sensitive, peaking at ~420 nm) cones^{2,4}. Rods allow humans to see at lower light levels (typically during nighttime), taking over from cones who perform poorly in these conditions. They do not populate the fovea (i.e., are most present in the periphery of the retina), do not contribute to colour vision, and peak at ~498 nm⁴.

By contrast, non-visual functions are mediated by the aforementioned ipRGCs. The ipRGCs are most sensitive to stimulation at ~480 nm⁴. The photopigment they contain, melanopsin, was first identified in the late 1990s, and subsequent works demonstrated its many functions in regulating human physiology, behaviour, and cognition^{1,2,5,6}. There is an increasing body of evidence supporting the modulation of visual perception from melanopic input⁷⁻⁹, thereby challenging the classical, clear distinction of cones and rod (visual) functions versus ipRGC (non-visual) functions.

Given the different spectral sensitivities and range of operation of the different human photoreceptors, spectral composition and intensity matter when investigating brightness sensitivity and discomfort glare. Any light will stimulate multiple photoreceptor classes to some extent, but photoreceptors with more closely overlapping spectral sensitivity

functions will tend to be more strongly co-activated by the same spectrum. For instance, spectra with high melanopic stimulation will often also produce substantial rod-weighted stimulation. This is a critical point to keep in mind when investigating photoreceptor mechanisms, because an effect associated with a given α -opic metric should not automatically be interpreted as evidence for the isolated contribution of that photoreceptor class.

How sensitive one is to light can differ widely between subjects. Overall, factors such as genetic background, sex, age, chronotype, time of day or lens anatomy may play a role in determining light sensitivity^{10,11}. Eye properties, such as pre-receptoral selective filtering of the short-wave (blue) part of the visible spectrum, can shift peak sensitivity of photoreceptors. Macular pigments, populating the fovea, have been shown to vary in optical density by a factor of ten in young healthy adults, whereas the crystalline lens can also vary in a sizeable manner – in 20-to-39-year-old subjects, optical density (OD) at 410 nm ranged from 0.8 to 1.8 OD, and in 60-to-80-year-olds, who are more exposed to lens yellowing, the spread of lens absorbance was even larger (up to 3.3 OD)¹². Ocular media also acts as an additional, short-wave light filter. All these differences need to be carefully considered and accounted for when running such studies.

While the physiological processes need to be understood, pathological conditions may equally be of interest to investigate the mechanistic underpinnings of light sensitivity and visual discomfort. People suffering from migraine often experience photophobia, manifesting an aversive response to light exposure typically way below the usual threshold for light discomfort observed in healthy individuals¹³. The proposed mechanism here is light-induced activation of the trigeminal nerves at the level of the trigeminal ganglion, in turn significantly deranging vascular function leading to pain^{13,14}. Rod monochromats do not have functional cones, forcing their visual system to rely solely on rods, which leads them to total colour blindness and photophobia. The latter occurs through rod saturation and absent cone-mediated adaptation¹⁵. Another phenomenon of interest is sneezing in response to bright light exposure, referred to as the photic sneeze reflex, photic sneeze syndrome, or Autosomal Dominant Compelling Helioophthalmic Outburst (ACHOO) syndrome, reportedly affecting up to 20 to 30% of the population^{16,17}. One hypothesis explaining its occurrence is that the reflex involves a genetically determined crosstalk between the visual and trigeminal pathways^{18,19}, and photic sneezers are also interestingly more susceptible to suffer from migraine, suggesting potential mechanistic similarities between the two conditions¹⁴.

Visual discomfort conventionally refers to a range of subjective and objective responses to different dimensions of visual stimulation, rather than a single uniform outcome. These

dimensions include responses to brightness, stripey or repetitive spatial patterns, strobing or motion, and visually intense environments, such as supermarkets²⁰. Some aspects of visual discomfort have been operationalised more specifically as glare. Disability glare refers to light-induced impairment of vision and reduced visibility, whereas discomfort glare refers to an unpleasant or painful sensation caused by light without necessarily reducing visual performance²¹. Importantly, it remains unclear whether these different discomfort responses reflect a common underlying mechanism or partly distinct mechanisms. The present study therefore focuses on controlled light-evoked responses to parametrically varied spectral and intensity properties, rather than treating visual discomfort as a single global construct.

To our knowledge, no studies have operationalised visual discomfort using simultaneous pupillometry, facial surface electromyography (sEMG), and self-reporting measurements, and we identify this as a research gap to fill. In this study (Figure 1), we will clarify the specific neural pathways and mechanisms underlying some of these various aspects of visual discomfort and the contribution of each photoreceptor type (rods, cones and ipRGCs) to these responses by using a combination of objective and subjective proxies of visual discomfort as a response to narrowband light of varying spectra under mesopic and photopic levels in controlled, laboratory conditions.


Our hypotheses are the following:

- Confirmatory CH₁: We hypothesise that the spectral sensitivity of light-adapted pupillary responses, i.e. pupillary light reflex (PLR) is best fit by melanopsin.
- Confirmatory CH₂: We hypothesise that the spectral sensitivity of EMG-measured squint is best fit by melanopsin.
- Exploratory EH₁: We hypothesise that the spectral sensitivity of scale-measured visual discomfort is best fit by melanopsin.
- Exploratory EH₂: We hypothesise that the spectral sensitivity of scale-measured facial sensations is best fit by melanopsin.


A note on terminology: In this report, “melanopic” and “rhodopic” refer to the corresponding α -opic spectral sensitivity functions of the CIE standard observer, not to isolated molecular absorption spectra of melanopsin or rhodopsin. The equivalent daylight illuminance (EDI) metrics used in this report are based on the CIE S 026:2018 international standard²², which built on the α -opic framework proposed by Lucas and colleagues⁴ and defines standardised α -opic spectral sensitivity functions for the five retinal photoreceptor classes. In this framework, EDI expresses the illuminance of

standard daylight that would produce the same α -opic irradiance as the test light. Thus, EDI metrics provide standardised, photoreceptor-specific descriptions of the effective stimulation produced by a given spectrum.


A. Experimental setup

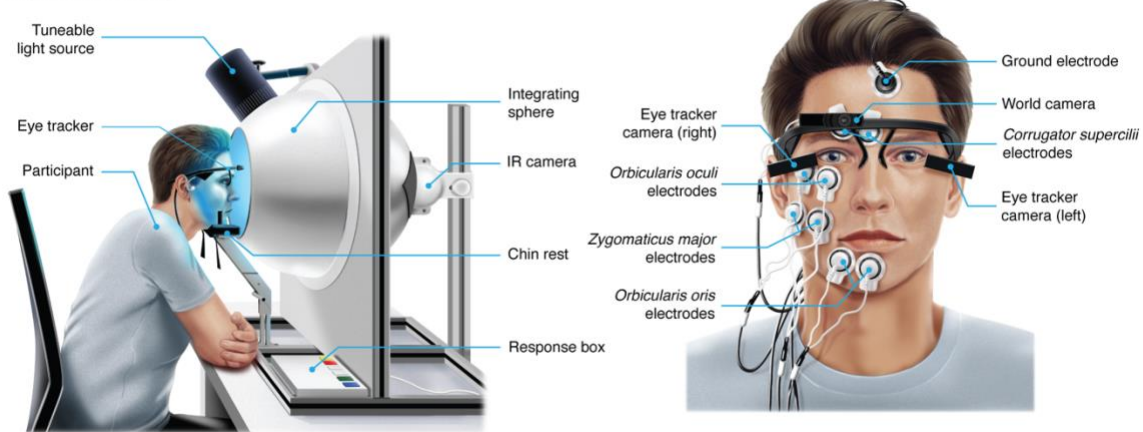

B. Experiment procedure

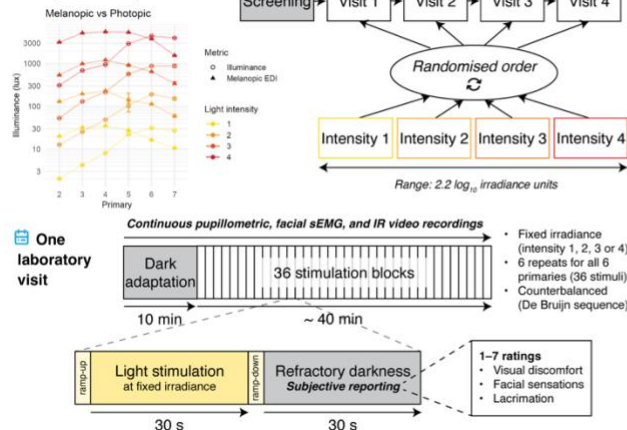

C. Stimulus properties

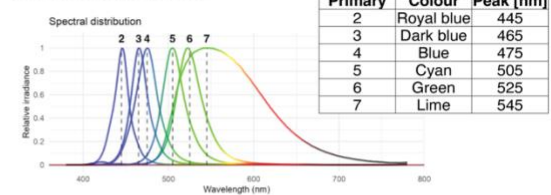

D. Research question and hypothesis

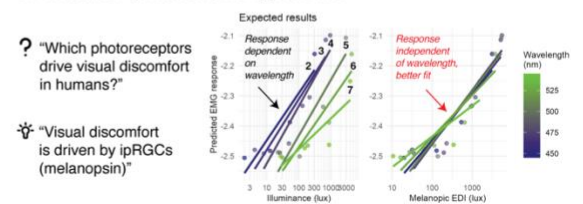


Figure 1. Overview of study design. (A) Participants sit in front of an integrating sphere and rest their head on a chin rest. A spectrally tuneable, 10-primary LED light source shines light into the sphere from above. While participants are exposed to light, binocular pupillometry, facial sEMG and infrared (IR) video recordings are performed. For sEMG, bipolar electrodes capture the electrical activity of four facial muscles on the right side of the face: corrugator supercilii, orbicularis oculi, zygomaticus major and orbicularis oris (sometimes impossible, due to e.g. beard). (B) Participants enrol for four laboratory visits, including a screening session during the first visit to confirm eligibility. One visit consists of 10 min of dark adaptation followed by 36 stimulation blocks. Each stimulation consists of a 3-s linear ramp-up, a 30-s light stimulation phase, a 3-s linear ramp-down, and a 30-s refractory darkness period, during which participants report their subjective experience of visual discomfort, facial sensations, and lacrimation using ratings on a 1-7 integer scale. Each of the four visits is randomly assigned a fixed irradiance from four possible values, assigned to all the stimuli regardless of the wavelength. This allows to present stimuli with varying ratios of melanopic, photopic and rhodopic stimulation, exposing the photoreceptors mechanisms at play in the measured responses. (C) The light stimuli have 6 different set wavelengths, spanning most of the short and medium part of the visible spectrum, with peaks from 445 to 545 nm. (D) We formulate the hypothesis that an ipRGC-tuned metric such as melanopic EDI (weighted to melanopsin sensitivity) provides a better fit than an L+M-

170 cone-tuned metric such as (photopic) illuminance when predicting visual discomfort responses. This would
171 mean that using illuminance as a predictor of visual discomfort does not capture the whole mechanisms at
172 play, leaving the responses dependent on stimulus wavelength. Using melanopic EDI as a predictor would,
173 on the other hand, fully and reliably characterise the measured visual discomfort responses.

174

Methods

Ethics information

This study complies with all relevant ethical regulations and has received ethical approval from the Technical University of Munich Ethics Committee. During the in-person screening, participants will provide written informed consent before any experimental procedures. The study will be performed in line with the principles of the Declaration of Helsinki. Participants will receive remuneration for their time – the details of which are described in the *Sampling plan* section.

Pilot data

A pilot study was designed and carried out to assess the feasibility of the protocol and inform Stage 1 of this Registered Report. The aim was to obtain data to characterise the dose-response curves for the modalities of interest, fit models to the data, and use these models to perform a fixed-n sensitivity analysis to determine the ability of this spectral sensitivity study to discriminate between melanopic, photopic, and rhodopic-driven orbicularis oculi EMG responses. The details and results of which are detailed in the *Sample size calculation* section.

The pilot study followed a similar design as the one described in the following sections – the deviations from this protocol are described in Table 1. Given the hypotheses tested in this spectral sensitivity study were already formulated, the pilot data was collected using white light of a correlated colour temperature (CCT) of 5000 K – not narrowband lights, to avoid data overlap and redundancy, therefore reducing bias when designing the final protocol, as formulating hypotheses after analysing data from the exact same protocol would go against the purpose of preregistering the study. It also allows generation of diverse data which may provide distinct information and insights into the mechanisms at play. The spectral power distributions (SPD) of all light conditions for both the pilot and main protocols are available in the *supplementary materials*.

206 *Table 1. Changes between the pilot and preregistered protocols*

Property	Pilot protocol	Final protocol
Number of laboratory visits	1	4
Stimuli	Varying intensity "White light": all 10 primaries on, constant spectra: CCT = 5000 K	Varying spectrum Individual primaries at fixed irradiance for each laboratory visit
Melanopic equivalent daylight illuminance (Melanopic EDI)	Range: 392 – 8408 lx → (~1.3 log ₁₀ units) + dark condition (0 lx)	Range: 10 – 5552 lx → (~2.7 log ₁₀ units)
Photopic illuminance	Range: 486 – 9821 lx → (~1.3 log ₁₀ units) + dark condition (0 lx)	Range: 2 – 4443 lx → (~3.3 log ₁₀ units)
Illuminance/Mel EDI ratio	Fixed ~1.2	Variable Range: 0.1 – 2.56 (~1.4 log ₁₀ units)
Irradiance range	Range: 1.6 – 35.6 W.m ⁻² → (~1.3 log ₁₀ units) + dark condition (0 W.m ⁻²)	Range: 0.06 – 8.8 W.m ⁻² → (~2.2 log ₁₀ units)

207
208 33 participants were recruited, and 22 were eligible to take part in the experiment. After
209 exclusion of incomplete or problematic data sets (due to electrodes disconnecting or
210 computer issues), 18 participants were finally included in the analysis of the EMG data.

211 The modality chosen for conducting the sensitivity analysis is the sEMG blinking/squinting
212 muscle (orbicularis oculi) activity. The rationale for using sEMG over pupillometry data is
213 that it constitutes the most reliable and stable outcome, using data loss as a proxy –
214 considered as the overall proportion of datasets where an issue arose during data
215 collection for each muscle. There was no data loss for the corrugator supercilii, around
216 5% for the orbicularis oculi, around 10 % for the zygomaticus major, and around 24% for
217 the orbicularis oris muscles. Pupillometric measurements, on the other hand, display from
218 29 % of data loss (expressed as the data lost during masking based on confidence at a
219 threshold of 0.7) at the lowest light level (392 mel EDI) to 77 % at the brightest light levels
220 (8408 mel EDI), on average, with high within-group variability. On a side note, there is on
221 average more pupillometry data loss at 0 lux than at 392 lux, since the pupil is bigger in
222 complete darkness and can be therefore harder to detect since its edges can be covered
223 by the eyelids. A visualisation of this data is available in the supplementary materials. The
224 sEMG data was preprocessed using the pipeline described in the *Analysis plan* section.

225 The orbicularis oculi muscle was chosen over the other facial muscles, since it was shown
226 to be the most reliable proxy for visual discomfort, and is not as sensitive to cognitive
227 input as the other viable candidate, the corrugator supercilii^{23–27}.

228

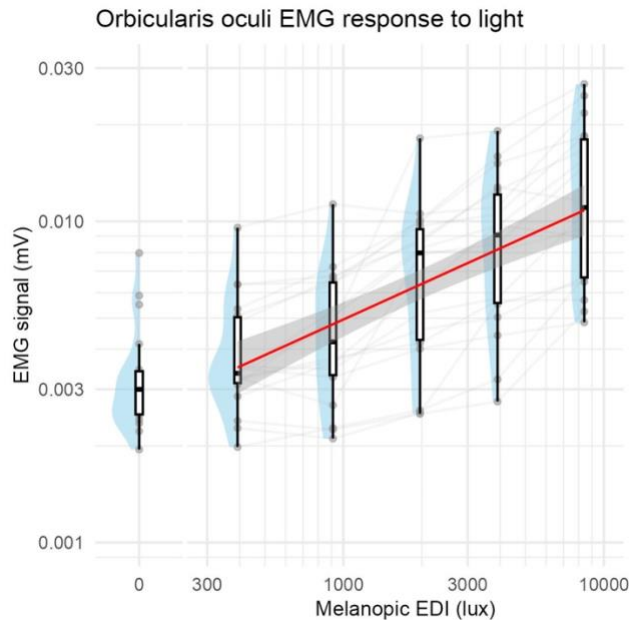


Figure 2. Dose-response curve of the orbicularis oculi (blinking/squinting) muscle sEMG response to light (melanopic EDI) after preprocessing, $n=18$. The red line shows linear fit to the non-0-lx data and the grey ribbon its 95% confidence interval.

For modelling, using a linear mixed model (LMM) was determined to be the best approach, because the data contain repeated measurements nested within participants, which induces correlations that ordinary linear regression cannot handle. The LMM allows each participant to have their own intercepts and/or slopes while still estimating a coherent group-level trend. This leads to more accurate uncertainty estimates, better handling of inter-subject variability, and a generative model that can simulate realistic new datasets with subject-specific variation.

The input and interaction of all different photoreceptor classes to the measured responses is of high relevancy and importance^{28–31}. Therefore, three models were fitted to the data, with either melanopic EDI, photopic illuminance, or rhodopic EDI as fixed effects. Under the fixed-spectrum design used here, changes in light intensity produced parallel changes in melanopic EDI, photopic illuminance, and rhodopic EDI, resulting in strong collinearity between these predictors and preventing their simultaneous inclusion in a single model.

The calculations were performed on R version 4.4.0³² using the *glmmTMB* R package version 1.1.14³³, specifically using the `glmmTMB()` function for model fitting.

The approach models the EMG response as a function of either melanopic EDI, illuminance, or rhodopic EDI ($\log_{10}$ transformed) while allowing for participant-dependent (random) slopes and intercepts, which can account for participant-level variation that may

otherwise be confounded with fixed effects of theoretical interest³⁴. Because of the $\log_{10}$ transformation, the 0-lux condition cannot be modelled directly, so an additional term Z_i was added. Z_i denotes a binary indicator variable, identifying whether the observation corresponds to the 0-lux condition (0), or one of the other, > 0-lux “light-on” conditions (1), essentially adjusting for lights on/off status. This allows to retain the baseline information (0-lux condition) in the modelling approach. Model comparisons based on Akaike’s Information Criterion (AIC)³⁵ revealed that adding trial number as well as baseline EMG signal (trial-level signal in the last second before lights turn on) meaningfully improved the model fit.

Regarding the rhodopic model, it might be of importance to note that rods are expected run into saturation^{36–39} at a certain level, so overall the actual relationship may actually be non-linear over the whole range of light levels (linear until saturation, then flat after saturation).

The final models were fitted with the following formula according to the Wilkinson-Rogers notation⁴⁰:

$$\log_{10}(\text{EMG signal}) \sim Z_i + \log_{10}(\text{Light exposure metric}) + \log_{10}(\text{Baseline EMG response}) + \text{Trial number} + (\log_{10}(\text{Light exposure metric}) | \text{Participant ID})$$

Because the spectral composition of the stimulus was held constant, melanopic EDI, rhodopic EDI, and photopic illuminance were near-perfectly correlated and represented alternative scalings of the same light-intensity manipulation. These models represent alternative parameterisations of light exposure and do not provide independent evidence for separable photoreceptor mechanisms. The reason for fitting three separate models is to subsequently use them as generative models during the sensitivity analysis described in the *Sampling plan* section – assuming either a melanopic-, photopic-, or rhodopic-driven response.

We report the full fixed-effect estimates for the primary melanopic EDI model – the two other models are reported in the *supplementary materials*. The linear mixed-effects model revealed a significant positive effect of melanopic EDI on the orbicularis oculi sEMG response ($p < 0.001$, $\beta = 0.354 \pm 0.015$, 95% CI [0.324, 0.384]), as well as a significant negative effect of Z_i ($p < 0.001$, $\beta = -0.884 \pm 0.040$, 95% CI [-0.963, -0.806]), a significant positive effect of the baseline EMG signal ($p < 0.001$, $\beta = 0.155 \pm 0.033$, 95% CI [0.090, 0.220]) and a significant, albeit small, effect of trial number ($p < 0.001$, $\beta = -0.002 \pm 0.000$, 95% CI [-0.003, -0.001]). The mixed-effects model included random intercepts for participants (SD = 0.126), and showed a marginal R^2 of 0.444, indicating that fixed effects explained 44.4% of the variance, and a conditional R^2 of 0.806, reflecting substantial

additional variance explained by participant-level random intercepts. Notably, marginal R^2 reflects variance partitioning within the full model rather than improvement over a random-effects-only baseline. Model diagnostics, computed using the `check_model()` function of the *performance* R package version 0.15.3⁴¹, including inspection of residual distributions, homogeneity of variance, influential observations, and deviations from linearity, are available in the *supplementary materials* as well as on the GitHub repository.

AIC values were highly similar across the melanopic EDI (-731.5), illuminance (-732.7), and rhodopic EDI (-731.3) models ($\Delta AIC \leq 2$), indicating near-equivalent model fit and supporting the interpretation that, under the fixed-spectrum stimulation used here, these metrics provided near-identical parameterisations of light intensity.

Table 2. Mixed-effects model output for the orbicularis oculi sEMG response to melanopic EDI.

Dependent variable			
Predictors	Estimates	CI	p
(Intercept)	-2.08	-2.25 – -1.91	<0.001
Z_i	-0.88	-0.96 – -0.81	<0.001
$\log_{10}$ (Melanopic EDI)	0.35	0.32 – 0.38	<0.001
$\log_{10}$ (Baseline EMG)	0.15	0.09 – 0.22	<0.001
Trial number	-0.00	-0.00 – -0.00	<0.001
Random effects			
σ^2	0.02		
T00 participant_id	0.02		
T11 participant_id.log_melanopic_edi	0.00		
ρ_{01} participant_id	-0.11		
ICC	0.65		
N participant_id	18		
Observations	648		
Marginal R^2 / Conditional R^2	0.444 / 0.806		

Design

In this study, each participant will be enrolling for a total of maximum five weeks, consisting of one initial meeting for screening, and four in-laboratory visits. The study design is within-subjects, testing the same participants across all conditions, and participants will be blinded to which conditions they are exposed to.

We will recruit healthy volunteers aged 18-35 years (to minimise differences in lens transmittance) for our within-subjects laboratory study taking place at the Max Planck Institute for Biological Cybernetics (Tübingen, Germany) across four one-hour experimental sessions. A sample size of 20 individuals was chosen, as resource limitations (money, time) prevent collecting data on more individuals. Within each session, light pulses from five narrowband wavelengths delivered through a spectrally tuneable LED (light-emitting diode) light engine (445, 465, 475, 505, 525, 545 nm) under homogenous, full-field stimulation at a fixed quantal radiance will be shown to participants in a counterbalanced sequence. Pupillometry and facial electromyography data will be recorded continuously (~120 Hz for pupillometry, 2048 Hz for the sEMG) during the trial, and subjective sensations (1-7 ratings for visual discomfort, facial sensations and lacrimation and associated confidence) reported. Prior to the sequence, participants undergo a ten-minute darkness adaptation period, followed by 36 trials of light stimulation, with each cycle consisting of 30 s of light exposure followed by 30 s of refractory darkness.

Timeline

During the first session, the participant will complete the screening to verify eligibility to participate according to the inclusion and exclusion criteria, as described in the *Sampling plan* section.

For each laboratory visit, participants will come at the same time-of-day, which they will decide (if possible), with measurements collected between 10:00 and 19:00. They will firstly be reminded of the instructions and the requirements to participate in the session.

At the beginning of each visit, they will complete a breathalyser and urine test, to ensure they are not under the influence of alcohol or drugs, and will report their subjective sleepiness. Next, the experimenter will set up the eye tracker and sEMG devices on the participant. The participants will be informed that the devices measure an eye response

only, to avoid cueing the participant to the measurements focusing on discomfort. After that, the experimenter will ask them to sit in front of the integrating sphere.

The experiment will then begin. The lights in the room will be switched off. Pupillometry, sEMG and infrared (IR) video measurements will be started, and participants will go through the initial 10-minute dark adaptation period.

The light stimulation will then begin. 36 stimuli blocks will occur in total. After each stimulation cycle, the participant will have to answer the subjective feedback questions using the response device with the help of auditory feedback. In total they will answer the questions 36 times, after each stimulus.

After the stimulation phase, the recordings will be stopped, the lights switched back on and the pupil tracker and sEMG devices taken off. Participants report again their sleepiness, after which the participant may leave the laboratory. They may also give consent to be contacted again for further studies during their last laboratory visit.

Light stimuli

Participants will be exposed to light stimuli differing in intensity and wavelength (spectral composition), sitting in front of the integrating sphere and resting their head on a chinrest (Figure 1). The participants will go through an initial 10-minute dark adaptation period, before presentation of the stimuli. Light exposure prior to the laboratory visits is not controlled for. To avoid fixational eye movements, participants will be asked to fixate a point in front of them at the back of the sphere during the entirety of the trial. The stimuli play in a counterbalanced manner, defined by a de Bruijn sequence⁴² – for each trial, the sequence is randomly chosen among a set of pre-generated counterbalanced sequences. The stimuli are presented as follows: a 3-second linear ramp-up, a 30-second plateau, a 3-second linear ramp down, and a 30-second refractory dark period. In this context, ‘linear’ refers to the control signal applied to the light source during the transition phases: the control signal is increased linearly from 0 to the target value over the 3-second ramp-up, and decreased linearly from the target value to 0 over the 3-second ramp-down. At each laboratory visit, participants will be shown light stimuli of one of four pre-set, log-spaced irradiance levels (0.06, 0.32, 1.6, 8.8 W.m⁻²), in a random order determined programmatically for each participant during their first laboratory visit. Light stimuli will be generated using the SpectraTune Lab (Ledmotive Technologies S.L., Barcelona, Spain) 10-primary LED light source. Six primaries (#2 to #7) will be used, with respective peak emissions at 445, 465, 475, 505, 525 and 545 nm. The primaries were chosen based on

their melanopic excitation potential. Each stimulus was calibrated so that so at each laboratory visit, all stimuli from the six primaries are of a fixed irradiance (measured horizontally at eye level out of the sphere), but of differing illuminance and melanopic EDI. The following design matrix summarises the described experimental approach. The calibration data, carried out using a Spectralval 1511 spectroradiometer from JETI Technische Instrumente GmbH, Jena, Germany, calibrated in October 2023 at the time the measurements were taken, as well as the design matrix and the corresponding completed ENLIGHT checklist⁴³, are available on the associated GitHub repository (https://github.com/tscnlab/BickerstaffEtAl_PCIRRStage1_2026).

Table 3. Light stimuli properties.

Lab visit	Primary	Peak [nm]	FWHM* [nm]	Colour	Light source setting (0-4095)	Irradiance [W/sqm] (380-780 nm)	Illuminance [lx]	Melanopic EDI [lx]	Melanopic to photopic ratio**
1	2	445	19	Royal blue	38	0.062	2.032	20.085	9.884
	3	465	23	Dark blue	49	0.066	4.243	31.823	7.500
	4	475	30	Blue	56	0.063	8.102	35.111	4.334
	5	505	30	Cyan	57	0.064	22.355	27.585	1.234
	6	525	34	Green	62	0.065	31.039	16.430	0.529
	7	545	110	Lime	52	0.071	27.247	10.654	0.391
2	2	445	19	Royal blue	128	0.354	12.670	129.534	10.224
	3	465	23	Dark blue	142	0.343	25.420	195.674	7.698
	4	475	30	Blue	156	0.350	49.043	230.240	4.695
	5	505	30	Cyan	166	0.283	111.794	147.206	1.317
	6	525	34	Green	174	0.346	191.183	113.174	0.592
	7	545	110	Lime	115	0.342	152.137	59.395	0.390
3	2	445	19	Royal blue	439	1.514	52.891	540.104	10.212
	3	465	23	Dark blue	537	1.703	130.209	991.170	7.612
	4	475	30	Blue	622	1.883	216.493	1207.548	5.578
	5	505	30	Cyan	454	1.583	573.437	915.052	1.596
	6	525	34	Green	577	1.654	876.532	647.720	0.739
	7	545	110	Lime	367	1.936	883.469	345.831	0.391
4	2	445	19	Royal blue	3230	8.731	310.267	3157.139	10.176
	3	465	23	Dark blue	3310	8.898	690.000	5175.748	7.501
	4	475	30	Blue	3511	8.802	950.813	5552.074	5.839
	5	505	30	Cyan	3196	8.884	2930.689	5366.997	1.831
	6	525	34	Green	4095	8.837	4443.253	3787.380	0.852
	7	545	110	Lime	1137	8.684	3979.285	1553.400	0.390

*FWHM: Full Width at Half Maximum

**Ratio of melanopic EDI divided by illuminance

Measurements

For each participant, all experiment sessions should be carried out at the same time of day, and if not possible, in the same time window during the day. The sessions may occur in time slots between 10:00 and 19:00.

Screening

Questionnaires

During the whole study, participants will complete a series of questionnaires and surveys, implemented in the REDCap (Research Electronic Data Capture) platform^{44,45}, hosted at the Technical University of Munich. REDCap is a secure, web-based software platform designed to support data capture for research studies, providing 1) an intuitive interface for validated data capture; 2) audit trails for tracking data manipulation and export procedures; 3) automated export procedures for seamless data downloads to common statistical packages; and 4) procedures for data integration and interoperability with external sources.

Chronotype

We will use the shortened version of the Munich Chronotype questionnaire (μ MCTQ)⁴⁶ to assess individual's biological predisposition for morning or evening times of day and its link to visual discomfort outcomes.

Light sensitivity

We will assess light sensitivity using two complementary tools. The first is the Visual Light Sensitivity Questionnaire (VLSQ-8)⁴⁷, measuring the presence and severity of visual photosensitivity symptoms, and the second the Cardiff Hypersensitivity Scale (CHYPS-V)⁴⁸, dividing the assessment into four factors (brightness, repeating patterns, strobing, and intense visual environments). The CHYPS-V will be used to distinguish brightness-related discomfort from other dimensions of visual sensitivity.

Sensory processing sensitivity

We will additionally use the Sensory Processing Sensitivity Questionnaire (SPSQ)⁴⁹, to assess general sensory sensitivity, to provide a bridge between the present visual-stimulus-focused design and overall sensory sensitivity.

Demographic variables

At screening, we will ask participants for their age, sex and gender identity.

Health variables

Physical health will be assessed using self-report questionnaires, aiming to screen for the variables described in the *Sampling plan* section.

Visual function

We will assess visual function using a variety of means. We will examine visual acuity using a Landolt C chart, and colour vision using HRR (Hardy Rand and Rittler)⁵⁰ plates (Richmond Products, Inc., Albuquerque, New Mexico, USA). The threshold for visual acuity is 20/40, which means 20/50 or worse on either eye will lead to exclusion from the study. The assessment will be made without any vision correction, because the eye tracking system prevents participants from wearing glasses, and contact lenses may affect corneal sensitivity. Excluding individuals wearing any glasses and contact lenses also makes recruitment more systematic and reliable.

Alcohol use

Participants will complete the Alcohol Use Disorders Identification Test (AUDIT)⁵¹, an instrument to examine substance and alcohol abuse, in the self-report version.

Reproductive status

Participants will complete a reproductive status questionnaire to determine their current hormonal functioning, and any hormonal medication intake.

Alcohol and drug tests

At the beginning of each laboratory evening, participants will be tested for alcohol and drug use. Participants will be asked to use a breathalyser (Alkoholtester ACE A, ACE Technik, Freilassing, Germany) to determine blood alcohol content (BAC). Participants will also be asked to produce a urine sample in a collection device, which will then be tested using a standard multi panel drug test (article number 620402, nal von minden GmbH, Moers, Germany) testing for amphetamines (1000 ng/mL cutoff), benzodiazepine (300 ng/mL cutoff), cocaine (300 ng/mL cutoff), morphine/opiates (300 ng/mL cutoff), and tetrahydrocannabinol (50 ng/mL cutoff). Should either test be positive, participants will not be able to participate that session.

Pupillometry measurements

Binocular pupillary data will be captured using the Pupil Core (Pupil Labs GmbH, Berlin, Germany) system⁵², an infrared video-based eye tracker recording at ~120 Hz. The data is collected using Pupil Capture version 3.5.7. The software uses an algorithmic approach to fit an ellipse to the detected 2D pupil and output a pupil size estimate in pixels, and fit a 3D eyeball model to the image to provide absolute pupil size in millimetres. There is a short calibration step ahead of the start of the dark period, where the participants are asked to look around, in all directions, for 30 seconds (more if needed), in order to allow the software to create a good model fit. The calibration step is recorded so that post-hoc pupil detection can be performed reliably (see *Analysis* plan section). Once the model is fit, it is frozen for the entire experiment. In this scenario, we assume that the slippage occurring during the experiment – potentially leading to a slightly inaccurate model towards the end of the trial – is preferable in comparison to not freezing the model, which allows constant correction in the model leading to relative differences in pupil size measurements from the start to the end, in turn making baseline correction inefficient. Participants will be instructed not to move their heads during the whole experiment, and keep focus on the IR camera at the back of the integrating sphere. This will be monitored and acted upon by orally reminding participants to do so should they not follow the instructions during data collection, using the live feedback of the eye cameras. The recording will take place in complete darkness, with the only light source being the IR lights from the IR camera. After the experiment, post-hoc pupil detection will be run on the eye video recordings using the Pupil Player software (version 3.5.7) as it may improve the quality of the data.

Facial surface electromyography measurements

Facial electromyography data will be captured using the EMG-USB2+ (OTBioelettronica SRL, Turin, Italy) system. It measures electrical signal of muscles in the face, interfacing with the experimental machine using the proprietary OTBiolab Light software (included in OTBiolab+ version 1.5.8) to allow collecting EMG data directly from a USB socket via Python. This device is used to measure facial muscle activity with a 16-channel bipolar adapter (AD8x2JD) and small bipolar electrodes. Here, four channels will be used for each of the corrugator supercilii, orbicularis oculi, zygomaticus major and orbicularis oris facial muscles. A gain of 1000 is applied to the signal. The ground electrode is placed in the centre on the forehead, just before the hairline. To maximise signal-to-noise ratio, the skin will be gently wiped with some abrasive paste to remove dead skin and increase skin conductance. The facial regions of interest (especially around the eye) are very sensitive and will therefore not be shaved by the experimenter. The zygomaticus major and orbicularis oris muscles may not be measured in bearded individuals as we will not ask them to shave for the purpose of the experiment. As facial muscle reactions to light exposure can be quite strong, tape will be applied on the electrodes to ensure they remain in position and measure accurately and consistently during the entire trial duration.

Subjective reporting

At the end of each light stimulation phase, participants will report their subjective sensations and associated confidence with a unified 1-7 integer rating scale, with 1 being the lowest and 7 the higher rating, using a MIDI device (Palette, Monogram, Kitchener, Ontario, Canada; controlled through the Monogram Creator Legacy version 4.1 software) which has knobs and buttons participants will use to report their ratings, with the help of automated auditory feedback. In total, participants give six ratings. First, they will report their visual discomfort – this is described as how uncomfortable the light they are being exposed to is making them feel. Then, they will rate their facial sensations – this is described as the intensity of the sensations (such as tickling, itching, burning...) they are getting in their face as a result of light stimulation. Finally, they report lacrimation – this is described as how much lacrimation has been generated in their eyes from the light they have just been exposed to. For clarity, lacrimation is also described as eye watering. For each of the three rating modalities, participants will also report an associated confidence rating – this is described as how confident they are in each of the ratings they just gave.

The Karolinska Sleepiness Scale (KSS) scale⁵³ (10-point version) will be used to measure the subjective level of sleepiness before and after each laboratory trial via self-reporting.

Video recordings

Faces of the participants will be recorded using an infrared camera (model number ALP-USBFHD05MT-DL36-DD-GM, ELP, Shenzhen, Guangdong, China) during the entirety of the trial, for participant monitoring purposes. The light sensor on the camera, which allows it to switch from RGB (Red, Green, Blue) to IR modes depending on ambient light levels, is blocked using tape, to keep the camera in IR mode permanently.

Software

The whole device control system is handled through a unified, custom Python module and controlled using the same experimental machine. The pupillometry system and light engine are controlled through Python using the PyPIr package⁵⁴ which offers an interface to Pupil Core⁵² and the SpectraTune Lab light source. Custom scripts were written for interfacing with the IR camera and EMG system. The latter collects timestamped data, which allows to synchronise the data stream with the pupillometry data (see *Analysis plan* section).

Sampling plan

Recruitment and screening

The aim of the present work is to examine how stimulus properties relate to visual discomfort in a broadly healthy sample, with no emphasis on clinical or high-sensitivity populations.

This study opts for a fixed-n design – recruitment will be run until 20 healthy adults have successfully completed the entire study, aiming for a balanced distribution of female and male biological sexes. Still, should $n=10$ be reached for one of the two sexes, participants will not be excluded from participating based on their sex. In the case subjects show very low data quality and need to be excluded based on the criteria laid down in the *Analysis plan* section, additional subjects will be recruited to reach the desired sample size.

Recruitment will follow multiple strategies, including advertising the study using flyers and posters displayed in authorised public places and on social media, using email lists and word-of-mouth.

Participants will have the choice to conduct the study in either German or English, depending on their preference. Participant-facing materials will be made available in both languages.

Participants will be given the opportunity to ask any questions before providing written consent to participate in the study.

Table 4. Inclusion criteria.

Domain	Criterion	Assessment method
Age	≥ 18 , ≤ 35 years of age	Self-report
Physical health	Good physical health	Self-report
Mental health	Good mental health	Self-report
Visual acuity	Normal visual acuity without correction	Landolt C chart (20/40 or better)
Colour vision	Normal colour vision	HRR plates

562 Table 5. Exclusion criteria.

Domain	Criterion	Assessment method
Vision correction	Wearing glasses or contact lenses	Self-report
Medication use	Any use of medications, including antihistamines	Self-report
Smoking	Habitual smoking	Self-report
Epilepsy	Diagnosis of epilepsy or family history of epilepsy	Self-report
Migraine	Diagnosis of migraine	Self-report
Recreational drug use	Use of recreational drugs	Self-report
Substance abuse	Excessive alcohol use	AUDIT
Allergies	Known allergies	Self-report
Acute drug screening	Presence of drugs	Multi-panel drug test

563

564 **Participant compensation**

565

566 Participants will be remunerated on the basis on EUR15 per hour. Considering each

567 session to be around one hour, and the initial meeting to be an hour too, participants can

568 be expected to spend a total of five hours in the laboratory as part of their participation in

569 the study, resulting in EUR75 of total remuneration.

570

571 **Sensitivity analysis**

572

573 A fixed-n sensitivity analysis was performed using simulated data, generated from the

574 three melanopic-, photopic-, and rhodopic-based model fits to the orbicularis oculi EMG

575 pilot data described in the *Pilot data* section of this manuscript. The aim was to determine

576 the ability of the experimental design to recover the assumed true driving mechanism

577 (melanopic, photopic, or rhodopic) given a fixed sample size of 20.

578 The calculation was performed on R version 4.4.0³² with the *glmmTMB* R package version

579 1.1.14³³, using the `glmmTMB()` function for model fits.

580

581 **Data simulation**

582

From this study's experimental design, a design matrix containing all conditions and associated melanopic EDI, illuminance, and rhodopic EDI (predictor) values determined through calibration spectral measurements (Table 3) was generated, needed to compute corresponding output EMG responses (outcome). Simulated datasets were generated from this experimental design matrix.

For each simulated dataset, fixed-effect predictions were generated from the selected generative model and participant-level random effects were drawn from the model-estimated random-effects variance-covariance structure. Residual error was then added using the residual standard deviation from the fitted generative model, electively multiplied by a prespecified noise-scaling factor. This allowed us to evaluate model recovery under both optimistic and pessimistic assumptions about residual variability. Baseline EMG values were simulated by empirical resampling from the observed pilot-study distribution of log-baseline values. For each simulation replicate, baseline values were resampled at the trial level.

Because the planned design extends to lower light levels than those observed in the pilot study, some simulated values fall below physiologically plausible baseline responses after extrapolation. Simulated observations for which the expected $\log_{10}$ response was below the fixed-effect prediction for the pilot study 0-lx condition (before adding residual error) were classified as non-physiological and excluded from model fitting. The amount of discarded data depends on the assumed generative driver, and this pattern is expected from the stimulus design, which emphasises the short-wavelength region and therefore preferentially favours melanopic and rhodopic stimulation relative to photopic stimulation. Therefore, the design matrix includes lower minimum photopic illuminance values than melanopic or rhodopic EDI values. Under a photopic generative model, these lower illuminance values make simulated responses more likely to fall below the physiological lower bound, leading to a higher proportion of discarded observations than under melanopic or rhodopic generative models. A floor was initially considered, which would allow retaining as much simulated data as possible. However, this would require modelling a non-linear response component in a region of the data space not supported by observed pilot data – unassigning data points from further consideration is therefore preferable to working with non-linear parameter estimates that have no basis in that region.

Model fitting and comparison

The sensitivity analysis included three runs – one run assuming a melanopic response driver (using melanopic-based generative model), one run assuming a photopic response driver (using illuminance-based generative model), and one run assuming a rhodopic response driver (using rhodopic-based generative model). Each run includes 1000 simulations.

For each simulation, three models are fitted – a “ m_{mel} ” model, a “ m_{phot} ” model, and a “ m_{rho} ” model. Predictor transformations matched those used in the fitted pilot models. The formula is as follows, using $\log_{10}$ -transformed light metric as the predictor variable and allowing for participant-dependent intercepts, according to the Wilkinson-Rogers notation⁴⁰:

$$\log_{10}(EMG\ signal) \sim \log_{10}(Light\ metric) + (1\ | \ Participant\ ID)$$

As a note, the Z_i parameter present in the modelling of the EMG pilot data (see *Pilot* data section) does not appear here as there is no 0-lux condition anymore in this protocol.

ΔAIC values are then calculated by comparing their AIC values, obtained as the difference between each model’s AIC and the lowest AIC within the three-model set³⁵. A model is considered as showing evidence for melanopic EDI, photopic illuminance, or rhodopic EDI when that model has the lowest AIC and all alternatives are more than 2 AIC units worse. If two or more models are within $\Delta AIC \leq 2$ of the best-fitting model, the comparison is judged to yield no clear preference.

The analysis was performed for a range of sample sizes (2 to 50) and noise scaling factor levels (0.5 to 10 times the residual noise when simulating data), indicating the conditions needed to properly capture the effect if it is present (a threshold of 0.8 for proportion of accurately recovered response driver is considered sufficient, which translates to an 80% chance of detection, given that the effect is true as parametrised).

Results

At $n=20$, the analysis indicated sufficient sensitivity (>0.8) up to noise levels 4 times greater than levels observed in the pilot data. Sensitivity naturally decreases as sample size becomes smaller and as noise increases – reflected by increasing proportions of comparisons yielding no clear preference. The sample size of $n=20$ is therefore deemed sufficient to detect the effect of interest provided it is true.

Collapsing across sample sizes and noise-scaling levels, the mean percentage of discarded observations was $50.98 \pm 0.14\%$ for simulations generated under the melanopic

model, $66.47 \pm 0.13\%$ for simulations generated under the photopic illuminance model, and $51.59 \pm 0.13\%$ for simulations generated under the rhodopic model. To assess whether the proportion of discarded simulated observations depended on simulation settings, we fitted a linear model predicting mean proportion of discarded data from assumed generative driver, sample size, and residual-noise scaling. After accounting for driver, there was no meaningful association with either sample size, $\beta = 1.69 \times 10^{-6}$, 95% CI $[-4.11 \times 10^{-6}, 7.48 \times 10^{-6}]$, $p = 0.568$, or noise scaling, $\beta = 6.10 \times 10^{-7}$, 95% CI $[-2.37 \times 10^{-5}, 2.49 \times 10^{-5}]$, $p = 0.961$. This indicates that the proportion of discarded observations was stable across sample-size and noise-scaling conditions, and was mainly determined by the assumed generative driver.

Model convergence rates were consistently high, at or nearing 100% for all sample sizes, noise levels, and assumed generative drivers.

The results and the diagnostics of the sensitivity analysis are available in the *supplementary materials* and on the associated GitHub repository.

Analysis plan

Software

For consistency, preprocessing and analyses of the data will be performed on Python 3.13⁵⁵ and R version 4.4.0³², building upon the existing pipeline developed for the pilot data.

Data preprocessing and outcome extraction

Pupillometry data pipeline

Before any analyses, the pupillary data is preprocessed using the following pipeline, which is applied separately on each recording of both eyes for each participant.

The eye tracking software outputs two pupil size metrics – 2D pupil size values in pixels, extracted from the frames only, and 3D pupil size values in millimetres, extracted from an eyeball model fit, which involves an extra computational step. Given that only relative changes are of interest for the purpose of this analysis, and that the extra computational step may introduce some extra error, 2D pupil size values will be used, predominantly for measurement reliability.

As mentioned in the *Pupillometry measurements* section, post-hoc pupil detection will be run on the eye video recordings, as it may improve the quality of the data. Also, for each participant, computations (preprocessing and analyses) are performed on one eye only, due to data quality considerations. The decision whether to use the left or right eye will be made programmatically on a participant level based on which data exhibits the less data loss after the confidence masking step.

The first preprocessing step is masking. The raw data is first filtered out using thresholds on the first derivative (± 0.5 standard deviations to the local mean, 5-sample window size). Then, a second filtering step is applied based on the confidence metric, which is an output quantifying certainty of measurement (0 = no confidence, 1 = perfect confidence). The eye tracking system manufacturer, Pupil Labs GmbH, states that pupil size values with associated confidence of 0.6 and above carry out useful information. In our case, the threshold is defined at the 60% quantile of all confidence values. This value needs to be

between 0.6 and 0.71, i.e. if the 60% confidence value quantile is 0.8, then it is lowered to 0.71, and if it is 0.45, then it is increased to 0.6. In our experience running similar protocols, excluding data with confidence above 0.71 poses a risk of discarding meaningful data. The approach here maximises data cleaning and preserves as much meaningful data as possible. Finally, a final masking step involves deleting physiologically impossible pupil size values, i.e. negative values. The data is then resampled to 60 Hz using linear interpolation – the raw pupillary data has a variable sample rate, usually around 120 Hz. A third-order polynomial Savitzky-Golay filter⁵⁶ is then applied to the resampled pupillary data, using a smoothing window of 61 samples (i.e., around 1 s at 60 Hz). Given how noisy the signal can be, resulting from participants squinting and blinking a lot making pupil detection harder, using a one second window helps with reducing noise, though at the expense of losing transient responses e.g., blinks. Divisive baseline correction is then applied to the pupil data. We select a global baseline tied to the dark period to be able to specify pupil responses to this absolute reference. The baseline pupil size corresponds to the median of the highest 10% pupil size values across the entire recording – for each participant and for each of the eyes. The median of the pupil size values during the last five minutes of the initial dark period was considered as a candidate for the baseline, but was found to be unreliable because of inconsistent pupil size measurements during dark period in the pilot study, with participants often dozing off or losing focus. Indeed, the best quality baseline pupil size data sometimes does not lie in the dark adaptation phase, but after, during the light stimulation cycles. A visual representation of all the data preprocessing steps for an example experiment run is available in the **Error! Reference source not found.**

The individual trial traces (time course -10 s before light onset to 30 seconds after light offset) are also kept for visualisation purposes.

What then follows is the calculation of participant-level averages of pupil constriction for each light condition and wavelength. The average pupil size during the 30-s plateau period is computed for all 36 trials of the four laboratory visits.

In addition to pupil size, pupil detection confidence, as reported by the eye tracking system, will be analysed as a secondary outcome. This confidence metric constitutes not only a technical index of measurement quality, but also an informative marker of whether the eye remains open and trackable during the stimulus, which may itself reflect an aversive ocular response to bright light. Confidence data will therefore be processed analogously to pupil-size data, including resampling to 60 Hz and smoothing with the same third-order Savitzky-Golay filter and 61-sample window. However, confidence values will not be masked on the basis of confidence itself. Individual trial-level confidence traces, spanning from 10 s before light onset to 30 s after light offset, will be retained for

visualisation of time-course dynamics. For each participant, light condition, and wavelength, average confidence during the 30-s plateau period will also be extracted across the 36 trials from the four laboratory visits.

EMG data pipeline

Before any analyses, the sEMG data is pre-processed using the following pipeline.

The data is first zero centred to correct for any DC (direct current) offset. Rectification is then applied by taking the absolute values of all data points. The rectified signal is low-pass filtered with a cutoff of 0.5 Hz normalised to the Nyquist frequency – $2048/2$ Hz – using a zero-phase (forward-backward), fourth-order Butterworth filter. 0.5 Hz corresponds to a 2-second period, so anything faster than a few seconds gets strongly suppressed – this choice was made on the basis that only the average EMG activity during light stimulation was of interest, and not transient responses (e.g. blinks). The sampling rate is kept high to preserve the raw signals as completely as possible, both for the present analyses and for future reuse of the data. Divisive baseline correction is then applied. The baseline corresponds to the median sEMG activity during the last five minutes of the initial dark period (i.e. five to ten minutes after the start of dark adaptation). A visual representation of all the data preprocessing steps for an example experiment run is available in the ***Error! Reference source not found.***

The individual trial traces (time course -10 s before light onset to 30 seconds after light offset) are also kept for visualisation purposes.

What then follows is calculation of participant-level averages of EMG activity for each light condition and wavelength. The average EMG activity during the 30-s plateau period is computed for all 36 trials of the 4 laboratory visits.

Subjective reporting data pipeline

The processing of rating data will involve the calculation of participant-level average ratings for each light condition and wavelength. A group average is finally computed for each rating for each combination of wavelength and light intensity.

Synchronisation of data streams

The time series data for pupillometry and EMG will be synchronised using the following strategy. The pupillary data serves as the reference in terms of timestamps, as the Pupil Capture software – alongside the PyPIr Python package⁵⁴ – supports the introduction of precisely-timestamped annotations in the recording (e.g. for marking the start of the experiment, the end of the initial dark adaptation period, or light onsets). The custom EMG Python software collects timestamped data separately, which allows to synchronise the data stream with the pupillometry data. All software is run on the same experimental machine, i.e. with a centralised clock for generating timestamps.

Data exclusion

In certain cases, datasets (i.e., pupillary data for one eye and for one participant) may be rejected upon the following criteria. Exclusion might result from issues during data collection – in cases where the experimenter reports relevant issues that may impact the reliability of the collected data, e.g. moving the eye tracker, or electrodes disconnecting during the experiment. Missing data would be the other reason – if the data presents obvious issues upon visual inspection, i.e., non-physiological responses, or, in the case of pupillometry data, if the percentage of remaining data after preprocessing falls below 10% of the original datasets (threshold defined from pilot data).

Statistical analysis

The same approach will be adopted here as the one described in the *Sample size calculation* section, where the data will be fit using LMMs and model fits compared using ΔAIC .

The calculation will be performed on R version 4.4.0³² using notably the *glmmTMB* R package version 1.1.14³³, using the `glmmTMB()` function for model fits.

For each outcome, three models are fitted – a “ m_{mel} ” model, a “ m_{phot} ” model, and a “ m_{rho} ” model. The response may be $\log_{10}$ -transformed should it be necessary. The formula is as follows, using $\log_{10}$ -transformed light metric as the predictor variable and allowing for participant-dependent intercepts, according to the Wilkinson-Rogers notation⁴⁰:

802
$$Response \sim \log_{10}(Light\ metric) + (1 \mid Participant\ ID)$$

803 As a note, the Z_i parameter present in the modelling of the EMG pilot data (see *Pilot data*
804 section) does not appear here as there is no 0-lux condition anymore in this protocol.

805 We will evaluate evidence for alternative spectral sensitivity models using AIC-based
806 model comparison³⁵. For each model set, ΔAIC will be calculated as the difference
807 between each model's AIC and the lowest AIC among the candidate models. Evidence
808 for the melanopic, photopic, or rhodopic model will be concluded when that model has
809 the lowest AIC and all alternative models are more than 2 AIC units worse. No clear
810 preference will be concluded when two or more models are within $\Delta AIC \leq 2$ of the lowest-
811 AIC model. These labels refer to relative empirical support for alternative spectral
812 sensitivity weightings and should not be interpreted as direct evidence for isolated
813 photoreceptor-specific mechanisms.

814 Any support for a specific model is limited to the wavelengths and exposure range tested
815 here. The findings will therefore be interpreted as evidence about which photoreceptor-
816 weighted metric best predicts responses within our stimulus set, not as evidence that a
817 given predictor provides a general account of visual discomfort under all spectral
818 conditions.

819

820

Relevance of reporting guidelines

The final report will aim, where feasible, to confirm to the following relevant reporting guidelines: the ENLIGHT checklist for light exposure documentation⁴³, the minimal reporting guideline for research involving eye tracking⁵⁷, the publication guidelines and recommendations for pupillary measurement in psychophysiological studies⁵⁸, and the guidelines for human electromyographic research⁵⁹.

Data availability statement

The data generated for this study will be made openly available on an online repository for free – Edmond (Max Planck Digital Library) – under an open license.

The complete pilot data set will be made available as part of another publication.

The data necessary to run the computations and generate the figures included in this manuscript are available on the GitHub repository associated with this Registered Report (https://github.com/tscnlab/BickerstaffEtAl_PCIRRStage1_2026).

Code availability statement

The code generated for this study will be made openly available on an online repository for free – GitHub – under an open license.

The code necessary to run the computations and generate the figures included in this manuscript are available on the GitHub repository associated with this Registered Report (https://github.com/tscnlab/BickerstaffEtAl_PCIRRStage1_2026).

AI use disclosure

The authors declare that ChatGPT (OpenAI) versions 5.2 and 5.5 – a Large Language Model (LLM) – is used as part of this research for the following matters:

- Generating, formatting, correcting and improving software code
- Generating small, isolated portions of text
- Correcting and formatting text

AI tools are not used to generate large portions of text (i.e. entire paragraphs) or illustrations.

Authors reviewed and edited all AI-assisted content, and carefully checked that there is no plagiarism, hallucinations or other errors. Authors take full responsibility for accuracy, originality, and interpretation.

Author contributions

We report author contributions using the CRediT taxonomy⁶⁰:

Conceptualisation: M.S., L.B., J.T., S.M.

Data curation (pilot study): L.B.

Formal analysis: L.B., J.Z., M.S.

Funding acquisition: M.S.

Investigation: L.B., J.T., M.S.

Methodology: L.B., M.S., J.Z., J.T., S.M.

Project administration: L.B., M.S.

Resources: M.S., L.B., J.T., S.M.

Software: L.B., J.Z.

Supervision: M.S.

874 Validation: L.B.
875 Visualisation: L.B., M.S., J.Z.
876 Writing – original draft: L.B.
877 Writing – review & editing: L.B., M.S., J.T., J.Z., S.M.
878

879 **Conflicts of interest**

880
881 L.B., J.T., and S.M. have no conflict of interest to declare.

882
883 J.Z. declares the following potential conflicts of interest in the past five years (2022-
884 2026).

885 **Academic roles:** Member of Joint Technical Committee 20 (JTC20) of the International
886 Commission on Illumination (CIE); Member of Research Data Alliance Working Group
887 Optical Radiation and Visual Experience Data; Speaker of group 2 (melanopic effects of
888 light) of the Technical Scientific Committee (TWA) of the German Society of Lighting
889 Technology and Design (LiTG)

890 **Remunerated roles:** Examiner, Swiss Lighting Society; Teacher, LiTG; Teacher,
891 University of Applied Sciences, Munich, Teacher, Technical University of Applied
892 Sciences, Rosenheim. Associated partner, 3lpi lighting design + engineering, Munich.
893 Tool- and 3D-model design, Zumtobel Lighting GmbH; Course design, University of
894 Applied Sciences, Munich & Virtual University Bavaria. Honoraria for talks: Received
895 honoraria from LiTG; Lamilux (Heinrich Strunz GmbH); Robert-Bosch Hospital Stuttgart;
896 Ergotopia GmbH; German statutory accident insurance institution for the administrative
897 sector (VBG); BRIXEN CULTUR, Italy; KITEO GmbH & Co.KG; University of Applied
898 Sciences Augsburg.

899 **Travel reimbursements:** Daimler und Benz Stiftung.

900 **Patents:** Together with 3lpi holds a design patent for non-visually optimized luminaire
901 (No 008194021-0001 through -0006) at the European Union Intellectual property office.

902 **Funding:** J.Z. position is funded by the "European Partnership on Metrology" with co-
903 funding from the "European Union's Horizon Europe Research and Innovation

Programme" and the participating member states; , *Wellcome Trust*, and *Reality Labs Research*.

M.S. declares the following potential conflicts of interest in the past five years (2021–2025):

Academic roles: Member of the Board of Directors, *Society of Light, Rhythms, and Circadian Health (SLRCH)*; Chair of Joint Technical Committee 20 (JTC20) of the *International Commission on Illumination (CIE)*; Member of the *Daylight Academy*; Chair of *Research Data Alliance Working Group Optical Radiation and Visual Experience Data*.

Remunerated roles: Speaker of the Steering Committee of the *Daylight Academy*; Ad-hoc reviewer for the *Health and Digital Executive Agency of the European Commission*; Ad-hoc reviewer for the *Swedish Research Council*; Associate Editor for *LEUKOS*, journal of the Illuminating Engineering Society; Examiner at the *University of Manchester*, *Flinders University*, and the *University of Southern Norway*.

Funding: Received research funding and support from the *Max Planck Society*, *Max Planck Foundation*, *Max Planck Innovation*, *Technical University of Munich*, *Wellcome Trust*, *National Research Foundation Singapore*, *European Partnership on Metrology*, *VELUX Foundation*, *Bayerisch-Tschechische Hochschulagentur (BTHA)*, *BayFrance (Bayerisch-Französisches Hochschulzentrum)*, *BayFOR (Bayerische Forschungsallianz)*, and *Reality Labs Research*.

Honoraria for talks: Received honoraria from *ISGlobal*, *Research Foundation of the City University of New York*, and the *Stadt Ebersberg, Museum Wald und Umwelt*.

Travel reimbursements: *Daimler und Benz Stiftung*.

Patents: Named on European Patent Application EP23159999.4A ("System and method for corneal-plane physiologically-relevant light logging with an application to personalized light interventions related to health and well-being").

With the exception of the funding source supporting this work, M.S. and J.Z. declare no influence of the disclosed roles or relationships on the work presented herein. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

References

1. Berson, D. M., Dunn, F. A. & Takao, M. Phototransduction by Retinal Ganglion Cells That Set the Circadian Clock. *Science* **295**, 1070–1073 (2002).
2. Blume, C., Garbazza, C. & Spitschan, M. Effects of light on human circadian rhythms, sleep and mood. *Somnologie* **23**, 147–156 (2019).
3. Mahoney, H. L. & Schmidt, T. M. The cognitive impact of light: illuminating ipRGC circuit mechanisms. *Nat. Rev. Neurosci.* **25**, 159–175 (2024).
4. Lucas, R. J. *et al.* Measuring and using light in the melanopsin age. *Trends in Neurosciences* **37**, 1–9 (2014).
5. Provencio, I., Jiang, G., De Grip, W. J., Hayes, W. P. & Rollag, M. D. Melanopsin: An opsin in melanophores, brain, and eye. *Proc. Natl. Acad. Sci. U.S.A.* **95**, 340–345 (1998).
6. Duda, M. *et al.* Melanopsin: From a small molecule to brain functions. *Neuroscience & Biobehavioral Reviews* **113**, 190–203 (2020).
7. Brown, T. M. *et al.* Melanopsin-Based Brightness Discrimination in Mice and Humans. *Current Biology* **22**, 1134–1141 (2012).
8. Cao, D., Chang, A. & Gai, S. Evidence for an impact of melanopsin activation on unique white perception. *J. Opt. Soc. Am. A* **35**, B287 (2018).
9. Zele, A. J., Adhikari, P., Feigl, B. & Cao, D. Cone and melanopsin contributions to human brightness estimation. *J. Opt. Soc. Am. A* **35**, B19 (2018).
10. Chellappa, S. L. Aging, light sensitivity and circadian health. *Aging* **13**, 25604–25606 (2021).

11. Spitschan, M. & Santhi, N. Individual differences and diversity in human physiological responses to light. *EBioMedicine* **75**, 103640 (2022).
12. Hammond, B. R. & Buch, J. Individual differences in visual function. *Experimental Eye Research* **199**, 108186 (2020).
13. Schulte, L. H., Allers, A. & May, A. Visual stimulation leads to activation of the nociceptive trigeminal nucleus in chronic migraine. *Neurology* **90**, (2018).
14. Sasayama, D. *et al.* Possible association between photic sneeze syndrome and migraine and psychological distress. *Neuropsychopharm Rep* **39**, 217–222 (2019).
15. Spitschan, M., Garbazza, C., Kohl, S. & Cajochen, C. Sleep and circadian phenotype in people without cone-mediated vision: a case series of five *CNGB3* and two *CNGA3* patients. *Brain Communications* **3**, fcab159 (2021).
16. Wang, M., Sun, X., Shi, Y., Song, X. & Mi, H. A genome-wide association study on photic sneeze reflex in the Chinese population. *Sci Rep* **9**, 4993 (2019).
17. Langer, N., Beeli, G. & Jäncke, L. When the Sun Prickles Your Nose: An EEG Study Identifying Neural Bases of Photic Sneezing. *PLoS ONE* **5**, e9208 (2010).
18. Everett, H. C. Sneezing in response to light. *Neurology* **14**, 483–483 (1964).
19. Trinkl, J., Bickerstaff, L., Munkwitz, S. & Spitschan, M. Stimulus conditions eliciting sneezing in response to bright light. *Exp Brain Res* **243**, 56 (2025).
20. Price, A., Sumner, P. & Powell, G. Understanding the subtypes of visual hypersensitivity: Four coherent factors and their measurement with the Cardiff Hypersensitivity Scale (CHYPS). *Vision Research* **233**, 108610 (2025).

- 980 21. Stiles, W. S. The scattering theory of the effect of glare on the brightness
981 difference threshold. *Proceedings of the Royal Society of London. Series B,*
982 *Containing Papers of a Biological Character* **105**, 131–146 (1929).
- 983 22. CIE. CIE S 026/E:2018 CIE System for Metrology of Optical Radiation for ipRGC-
984 Influenced Responses to Light. doi:10.25039/S026.2018.
- 985 23. Kaiser, E. A. *et al.* Reflexive Eye Closure in Response to Cone and Melanopsin
986 Stimulation: A Study of Implicit Measures of Light Sensitivity in Migraine. *Neurology*
987 **97**, (2021).
- 988 24. Hackley, S. A. & Johnson, L. N. The photic blink reflex as an index of
989 photophobia. *Biological Psychology* **184**, 108695 (2023).
- 990 25. Van Boxtel, A. & Jessurun, M. Amplitude and bilateral coherency of facial and
991 jaw-elevator EMG activity as an index of effort during a two-choice serial reaction
992 task. *Psychophysiology* **30**, 589–604 (1993).
- 993 26. Nahar, N. K., Gowrisankaran, S., Hayes, J. R. & Sheedy, J. E. Interactions of
994 visual and cognitive stress. *Optometry - Journal of the American Optometric*
995 *Association* **82**, 689–696 (2011).
- 996 27. Gowrisankaran, S., Sheedy, J. E. & Hayes, J. R. Eyelid Squint Response to
997 Asthenopia-Inducing Conditions. *Optometry and Vision Science* **84**, 611–619 (2007).
- 998 28. Uprety, S., Adhikari, P., Feigl, B. & Zele, A. J. Melanopsin photoreception
999 differentially modulates rod-mediated and cone-mediated human temporal vision.
1000 *iScience* **25**, 104529 (2022).

29. Schroeder, M. M. *et al.* The Roles of Rods, Cones, and Melanopsin in Photoresponses of M4 Intrinsically Photosensitive Retinal Ganglion Cells (ipRGCs) and Optokinetic Visual Behavior. *Front. Cell. Neurosci.* **12**, 203 (2018).
30. Altimus, C. M. *et al.* Rod photoreceptors drive circadian photoentrainment across a wide range of light intensities. *Nat Neurosci* **13**, 1107–1112 (2010).
31. Lamb, T. D. Why rods and cones? *Eye* **30**, 179–185 (2016).
32. R Core Team. *R: A Language and Environment for Statistical Computing*. (R Foundation for Statistical Computing, Vienna, Austria, 2024).
33. McGillicuddy, M., Warton, D. I., Popovic, G. & Bolker, B. M. Parsimoniously Fitting Large Multivariate Random Effects in **glmmTMB**. *J. Stat. Soft.* **112**, (2025).
34. Barr, D. J., Levy, R., Scheepers, C. & Tily, H. J. Random effects structure for confirmatory hypothesis testing: Keep it maximal. *Journal of Memory and Language* **68**, 255–278 (2013).
35. *Model Selection and Multimodel Inference*. (Springer New York, New York, NY, 2004). doi:10.1007/b97636.
36. Aguilar, M. & Stiles, W. S. Saturation of the Rod Mechanism of the Retina at High Levels of Stimulation. *Optica Acta: International Journal of Optics* **1**, 59–65 (1954).
37. Adelson, E. H. Saturation and adaptation in the rod system. *Vision Research* **22**, 1299–1312 (1982).
38. Tikidji-Hamburyan, A. *et al.* Rods progressively escape saturation to drive visual responses in daylight conditions. *Nat Commun* **8**, 1813 (2017).
39. Frederiksen, R. *et al.* Rod Photoreceptors Avoid Saturation in Bright Light by the Movement of the G Protein Transducin. *J. Neurosci.* **41**, 3320–3330 (2021).

- 1024 40. Wilkinson, G. N. & Rogers, C. E. Symbolic Description of Factorial Models for
1025 Analysis of Variance. *Applied Statistics* **22**, 392 (1973).
- 1026 41. Lüdtke, D., Ben-Shachar, M., Patil, I., Waggoner, P. & Makowski, D.
1027 performance: An R Package for Assessment, Comparison and Testing of Statistical
1028 Models. *JOSS* **6**, 3139 (2021).
- 1029 42. Aguirre, G. K., Mattar, M. G. & Magis-Weinberg, L. de Bruijn cycles for neural
1030 decoding. *NeuroImage* **56**, 1293–1300 (2011).
- 1031 43. Spitschan, M. *et al.* ENLIGHT: A consensus checklist for reporting laboratory-
1032 based studies on the non-visual effects of light in humans. *eBioMedicine* **98**, 104889
1033 (2023).
- 1034 44. Harris, P. A. *et al.* Research electronic data capture (REDCap)—A metadata-
1035 driven methodology and workflow process for providing translational research
1036 informatics support. *Journal of Biomedical Informatics* **42**, 377–381 (2009).
- 1037 45. Harris, P. A. *et al.* The REDCap consortium: Building an international community
1038 of software platform partners. *Journal of Biomedical Informatics* **95**, 103208 (2019).
- 1039 46. Ghotbi, N. *et al.* The μ MCTQ: An Ultra-Short Version of the Munich ChronoType
1040 Questionnaire. *J Biol Rhythms* **35**, 98–110 (2020).
- 1041 47. Verriotto, J. D. *et al.* New Methods for Quantification of Visual Photosensitivity
1042 Threshold and Symptoms. *Transl Vis Sci Technol* **6**, 18 (2017).
- 1043 48. Price, A., Sumner, P. & Powell, G. Understanding the subtypes of visual
1044 hypersensitivity: Four coherent factors and their measurement with the Cardiff
1045 Hypersensitivity Scale (CHYPS). *Vision Research* **233**, 108610 (2025).

49. Malinakova, K., Novak, L., Trnka, R. & Tavel, P. Sensory Processing Sensitivity Questionnaire: A Psychometric Evaluation and Associations with Experiencing the COVID-19 Pandemic. *IJERPH* **18**, 12962 (2021).
50. Hardy, L. H., Rand, G. & Rittler, M. C. H–R–R Polychromatic Plates*. *J. Opt. Soc. Am.* **44**, 509 (1954).
51. Saunders, J. B., Aasland, O. G., Babor, T. F., De La Fuente, J. R. & Grant, M. Development of the Alcohol Use Disorders Identification Test (AUDIT): WHO Collaborative Project on Early Detection of Persons with Harmful Alcohol Consumption-II. *Addiction* **88**, 791–804 (1993).
52. Kassner, M., Patera, W. & Bulling, A. Pupil: an open source platform for pervasive eye tracking and mobile gaze-based interaction. in *Proceedings of the 2014 ACM International Joint Conference on Pervasive and Ubiquitous Computing: Adjunct Publication* 1151–1160 (ACM, Seattle Washington, 2014). doi:10.1145/2638728.2641695.
53. Shahid, A., Wilkinson, K., Marcu, S. & Shapiro, C. M. Karolinska Sleepiness Scale (KSS). in *STOP, THAT and One Hundred Other Sleep Scales* (eds Shahid, A., Wilkinson, K., Marcu, S. & Shapiro, C. M.) 209–210 (Springer New York, New York, NY, 2011). doi:10.1007/978-1-4419-9893-4_47.
54. Martin, J. T., Pinto, J., Bulte, D. & Spitschan, M. PyPIr: A versatile, integrated system of hardware and software for researching the human pupillary light reflex. *Behav Res* **54**, 2720–2739 (2021).
55. van Rossum, G. & de Boer, J. Interactively testing remote servers using the Python programming language. *CWI Quarterly* **4**, 283–304 (1991).

- 1069 56. Savitzky, Abraham. & Golay, M. J. E. Smoothing and Differentiation of Data by
1070 Simplified Least Squares Procedures. *Anal. Chem.* **36**, 1627–1639 (1964).
- 1071 57. Dunn, M. J. *et al.* Minimal reporting guideline for research involving eye tracking
1072 (2023 edition). *Behav Res* **56**, 4351–4357 (2023).
- 1073 58. Steinhauer, S. R., Bradley, M. M., Siegle, G. J., Roecklein, K. A. & Dix, A.
1074 Publication guidelines and recommendations for pupillary measurement in
1075 psychophysiological studies. *Psychophysiology* **59**, e14035 (2022).
- 1076 59. Fridlund, A. J. & Cacioppo, J. T. Guidelines for Human Electromyographic
1077 Research. *Psychophysiology* **23**, 567–589 (1986).
- 1078 60. NISO CRediT Working Group. ANSI/NISO Z39.104-2022, CRediT, Contributor
1079 Roles Taxonomy. doi:10.3789/ansi.niso.z39.104-2022.

Table 6. Study design template

Question	Hypothesis	Sampling plan	Analysis plan	Rationale for deciding the sensitivity of the test for confirming or disconfirming the hypothesis	Interpretation given different outcomes	Theory that could be shown wrong by the outcomes
What photoreceptor mechanisms underlie subjective and objective physiological responses to bright light in humans?	We predict that the spectral sensitivity of physiological responses (pupillometry outcomes, EMG outcomes, subjective reporting outcomes) to bright light is better fit by melanopsin than by L+M opsins (photopic) or by rods (rhodopic).	20 participants will be recruited, sufficient as per sensitivity analysis	AIC-based model comparison, linear mixed models Fixed effects: The spectral sensitivity model was varied by replacing the light-exposure predictor with melanopic EDI, photopic illuminance, or rhodopic EDI. Random effects: Participant-specific random intercepts	<u>No clear preference: two or more candidate models are within $\Delta AIC \leq 2$ of the lowest-AIC model.</u> <u>Evidence favouring one model: one candidate model has the lowest AIC, and all alternative models are more than 2 AIC units worse.</u> <u>These categories indicate relative model support among the candidate spectral sensitivity models, not definitive evidence for isolated photoreceptor-specific mechanisms.</u>	If one spectral sensitivity model is favoured, this would indicate that physiological responses to bright light are best explained by the corresponding spectral sensitivity weighting among the candidate models. For example, evidence favouring the melanopic EDI model would support the interpretation that the measured responses are more consistent with melanopic than photopic or rhodopic sensitivity. If no model is clearly favoured, this would indicate that the candidate spectral sensitivity weightings provide equivalent explanations of the observed responses.	There is a growing body of evidence suggesting that melanopsin is the main driver of many visual functions, including visual discomfort. Our study will contribute to further characterise the biological system at play and, if the evidence is inconclusive, may suggest that melanopsin is only partially, or not all, involved in visual discomfort responses in humans.