

SpectraNova SN-4 plate reader calibration

Plate Reader / OCW-PL-017

Orchid Cellworks

Study Alpha

2026-07-13

cohort A-24

assay 6.8 ng/mL

Run: ALPHA-A24-R03

Slope: 0.998 R2: 0.9992

Status: ACCEPT					

Synthetic calibration record - no clinical or participant data

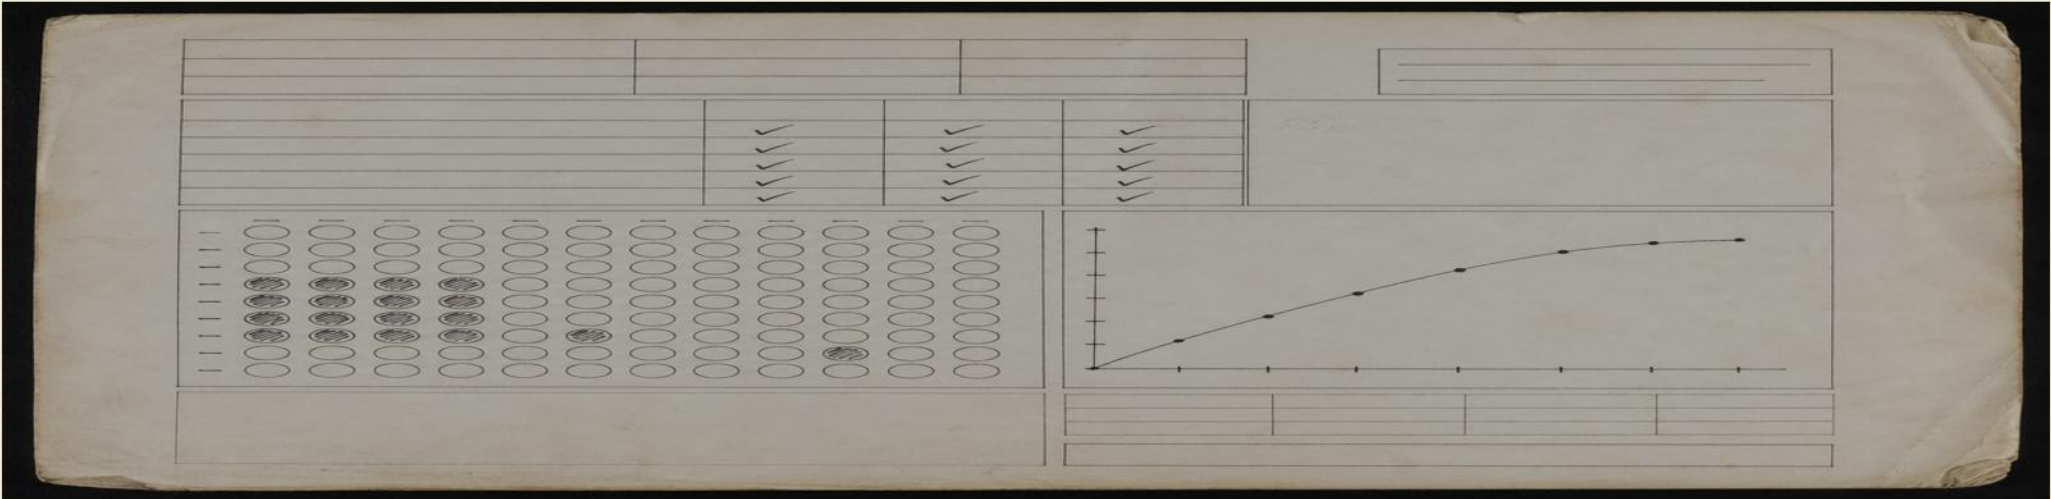


Image source: unique generated scan artwork; final review completed