

SpectraNova linearity check

Linearity / OCW-LN-009

Orchid Cellworks


Absorbance linearity check

2026-07-13

Range: 0.02 - 2.00 AU

R2: 0.9992

Status: ACCEPT

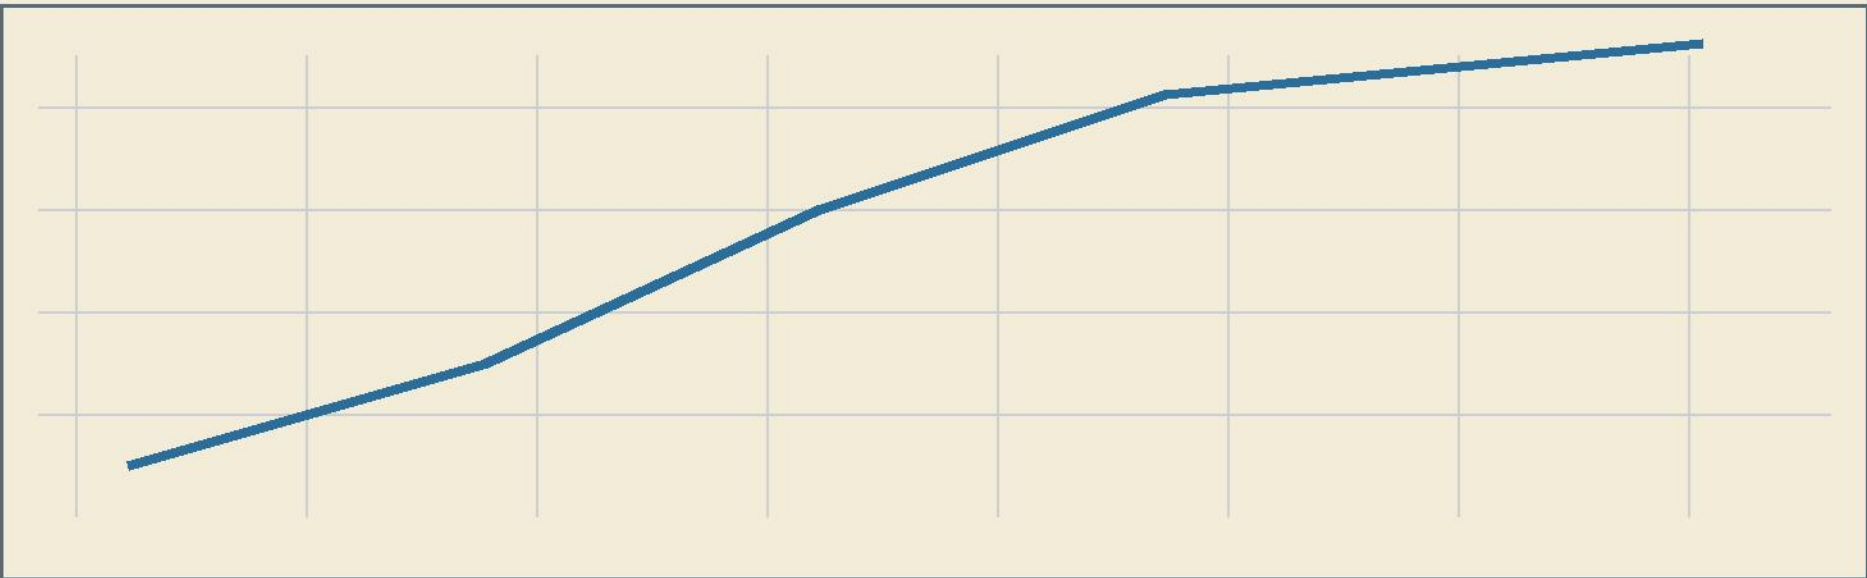

Synthetic calibration record - no clinical or participant data

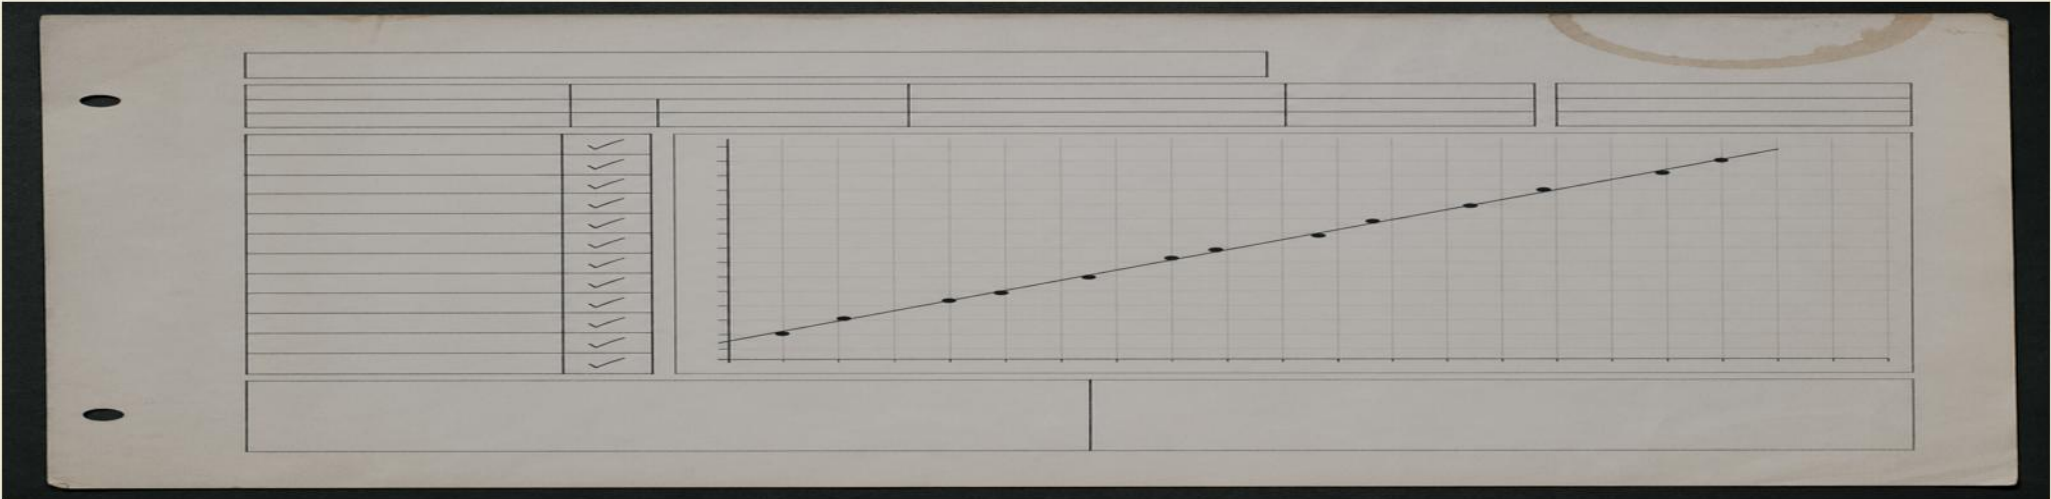


Image source: unique generated scan artwork; final review completed